


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072720\
 Data File : BF121033.D
 Acq On : 27 Jul 2020 15:36
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 14:20:32 2020

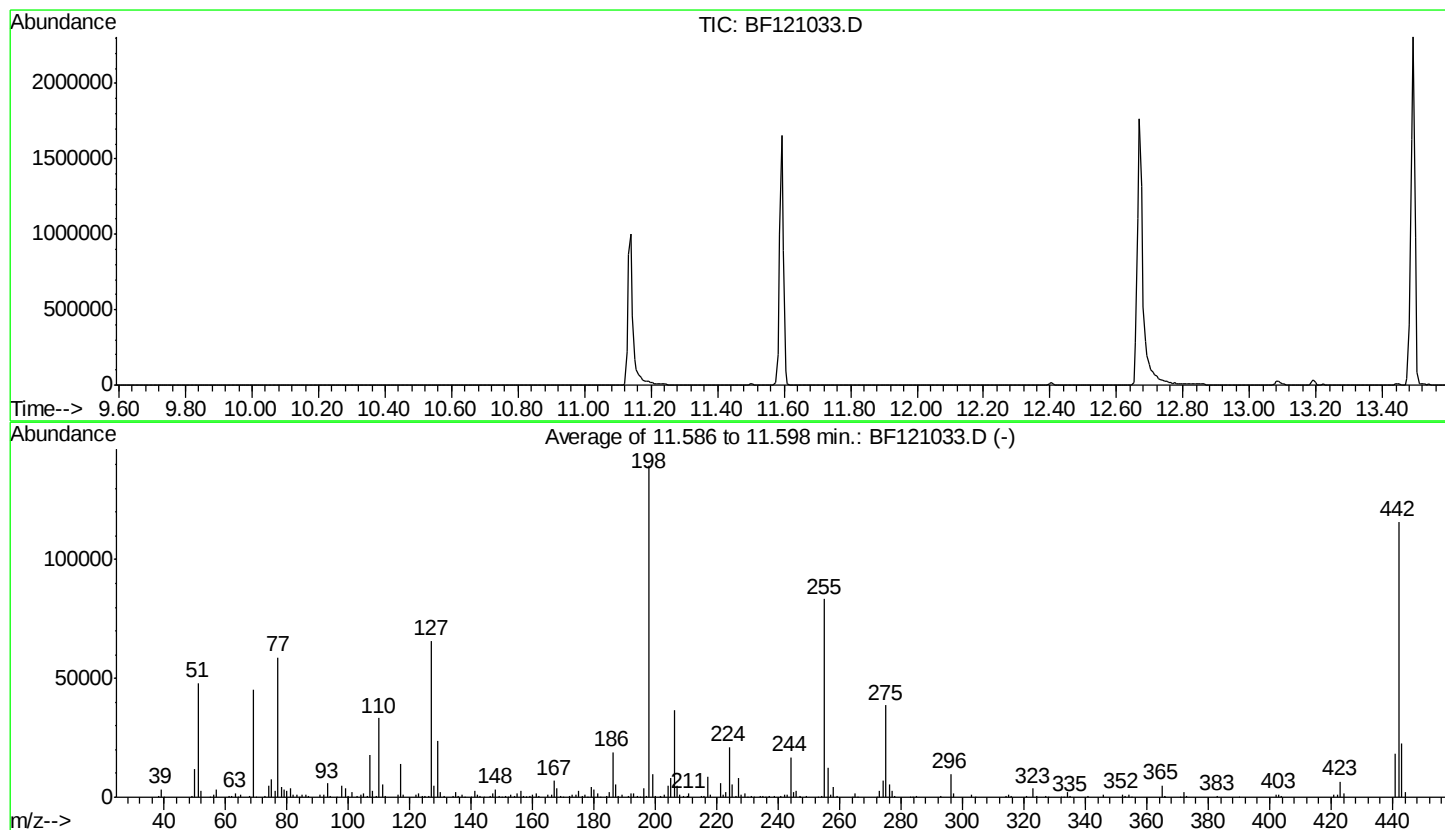

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	48248	PASS
68	69	0.00	2	1.7	756	PASS
69	198	0.00	100	32.5	45413	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	47.3	65970	PASS
197	198	0.00	2	0.6	784	PASS
198	198	100	100	100.0	139608	PASS
199	198	5	9	6.8	9508	PASS
275	198	10	60	27.7	38602	PASS
365	198	1	100	3.6	4997	PASS
441	198	0.01	100	13.1	18296	PASS
442	198	50	100	83.1	116072	PASS
443	442	15	24	19.3	22408	PASS