
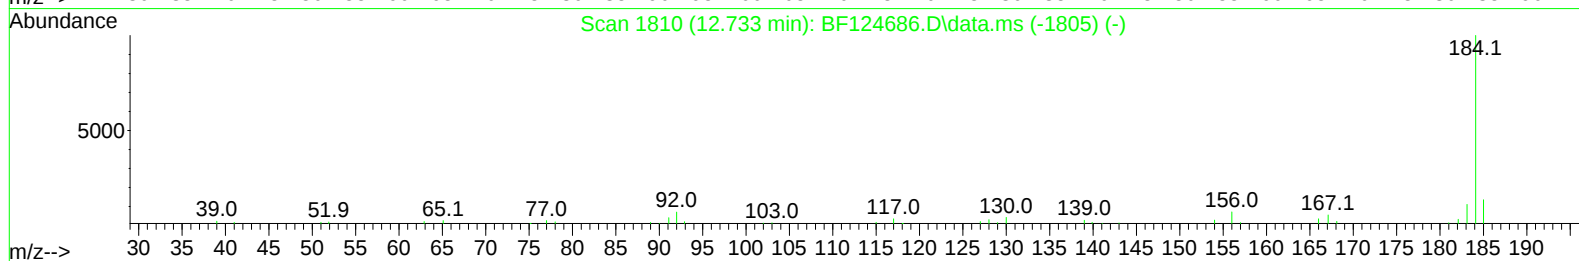
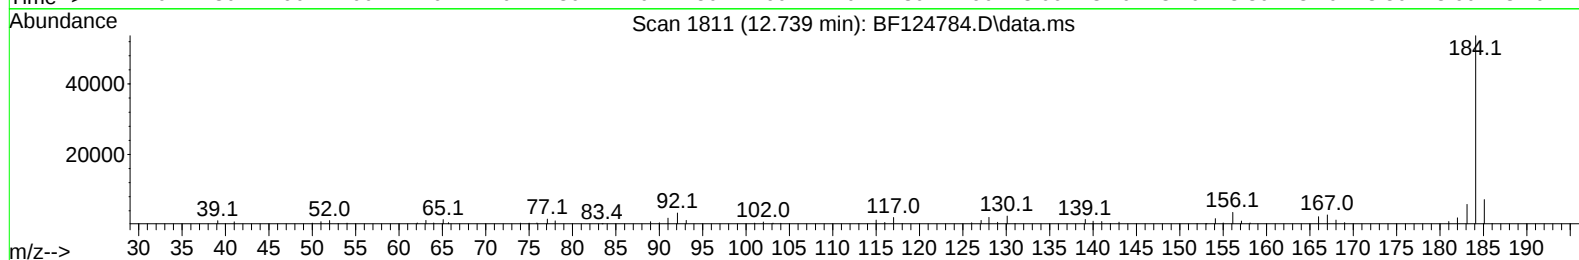


Quant Time: Jul 27 10:51:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

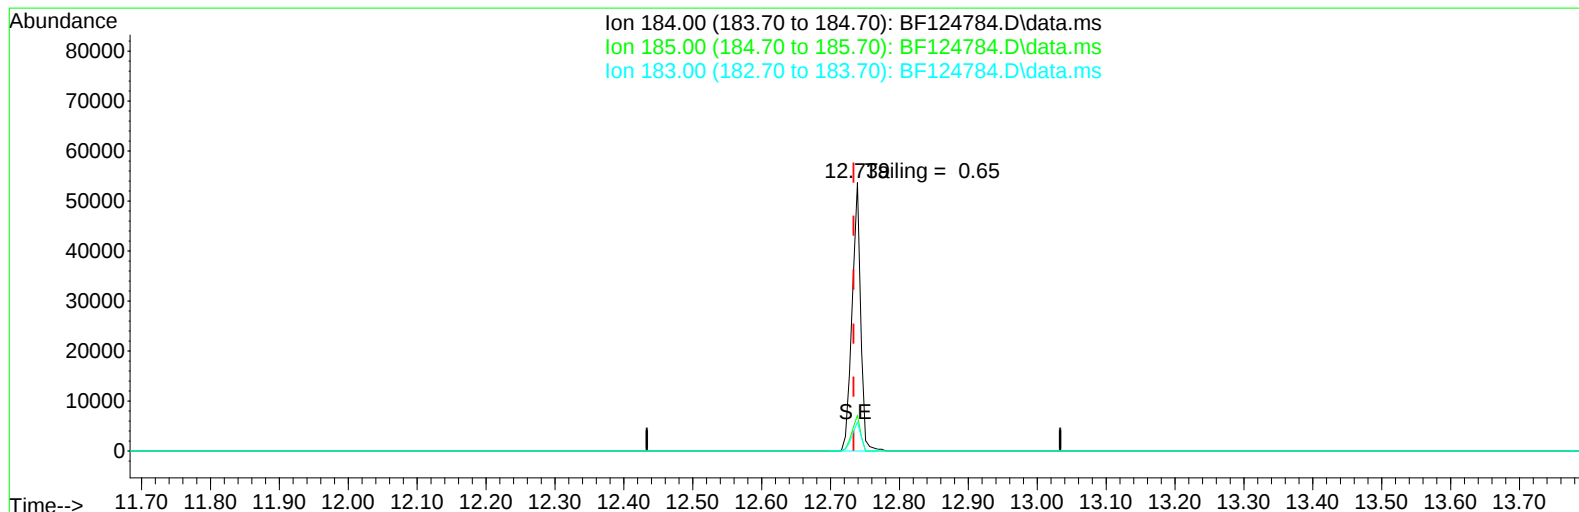

TIC: BF124784.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response **46523**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------




185.00	13.50	13.40
--------	-------	-------

183.00	10.10	10.80
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124784.D
Acq On : 27 Jul 2021 9:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 10:51:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

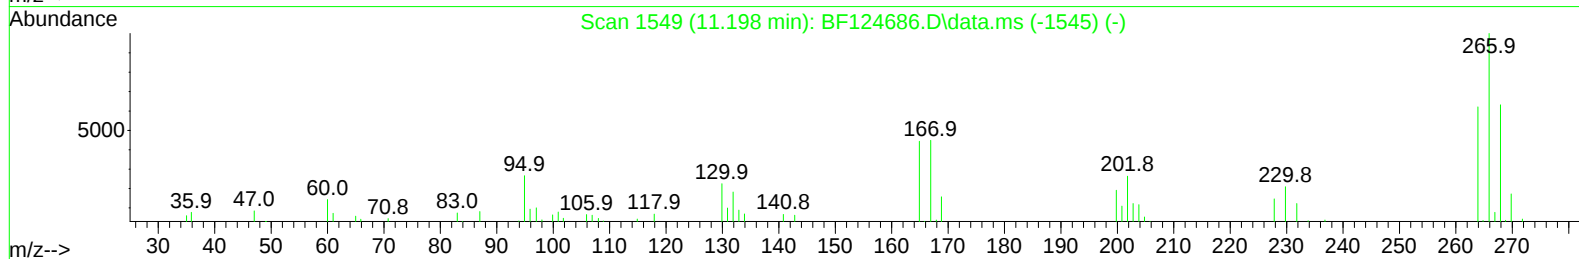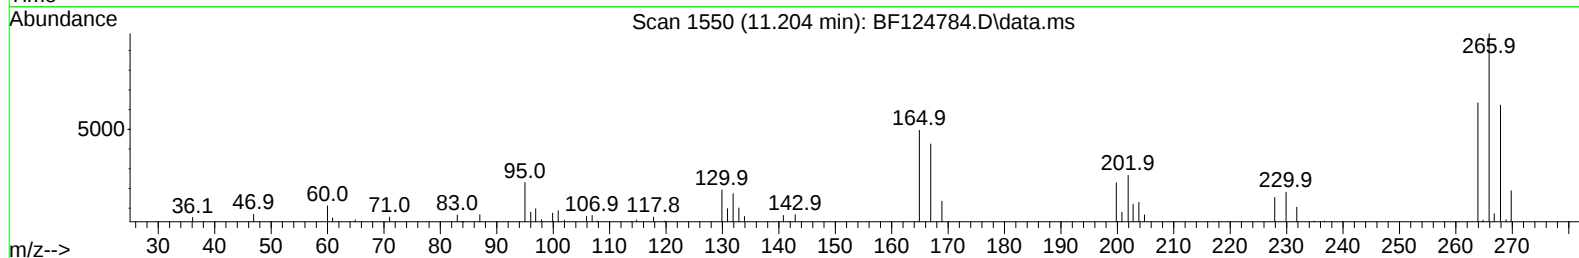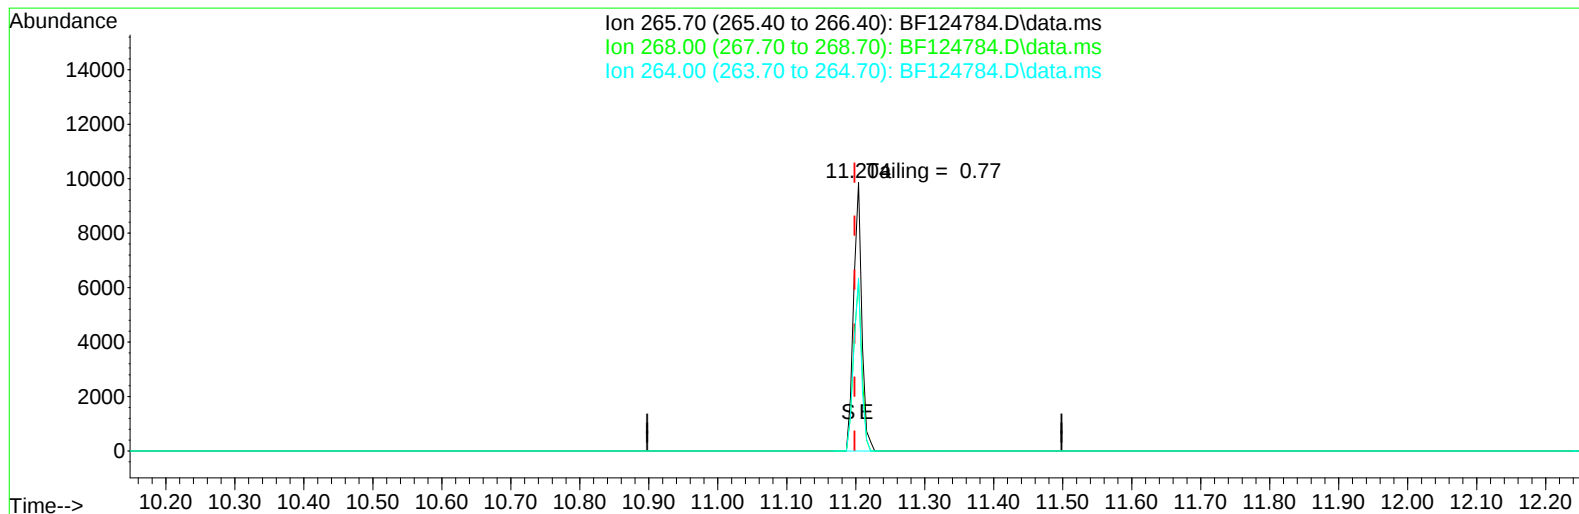

TIC: BF124784.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 0.00 ng

response 8147

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.20
264.00	69.90	64.36
0.00	0.00	0.00