

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
 Data File : BF124790.D
 Acq On : 27 Jul 2021 12:26
 Operator : JU/CG
 Sample : PB137900BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137900BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	576	581	584	rBB	216936	240305	63.37%	12.591%
2	6.504	745	751	754	rBB	210601	241301	63.63%	12.643%
3	6.869	810	813	816	rBB	53431	43567	11.49%	2.283%
4	7.439	904	910	912	rBB	136885	160797	42.40%	8.425%
5	8.151	1027	1031	1035	rBB	63715	60330	15.91%	3.161%
6	9.233	1209	1215	1218	rBV	324599	318869	84.08%	16.708%
7	9.910	1325	1330	1333	rBB	88223	73131	19.28%	3.832%
8	10.704	1459	1465	1468	rBV	212055	201143	53.04%	10.539%
9	11.398	1579	1583	1586	rBV	100927	77235	20.37%	4.047%
10	12.992	1848	1854	1857	rBV	393495	379223	100.00%	19.870%
11	14.039	2028	2032	2035	rBV	69799	63745	16.81%	3.340%
12	15.515	2278	2283	2288	rBB	39309	48873	12.89%	2.561%




Sum of corrected areas: 1908519

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124790.D
Acq On : 27 Jul 2021 12:26
Operator : JU/CG
Sample : PB137900BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137900BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

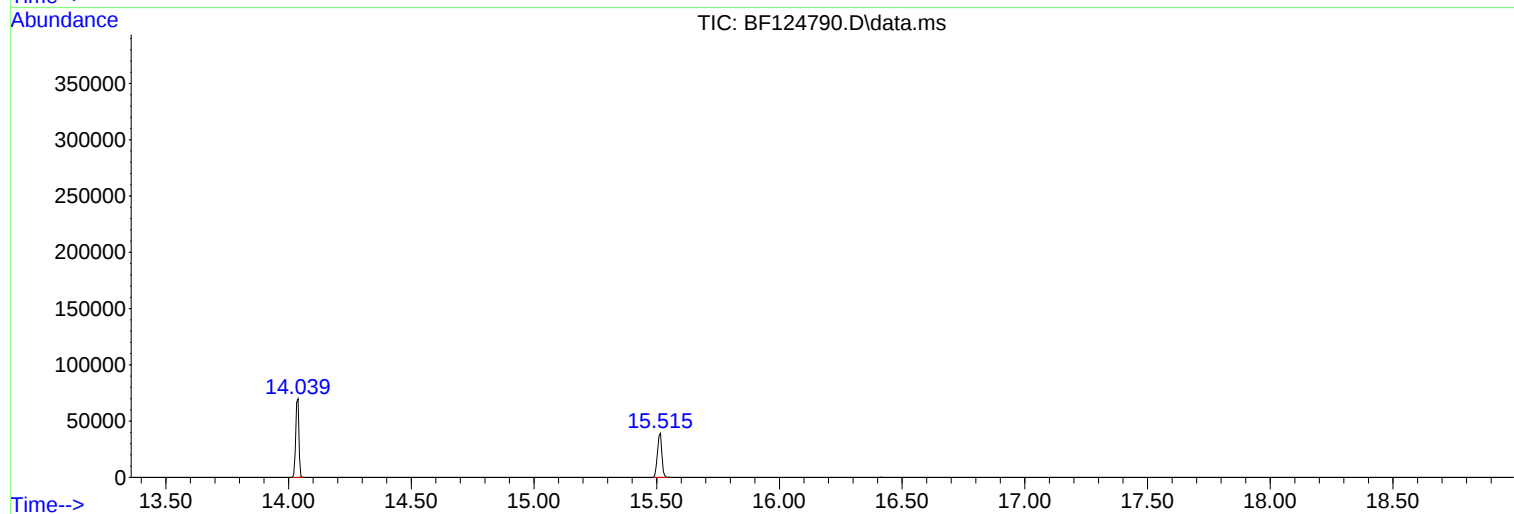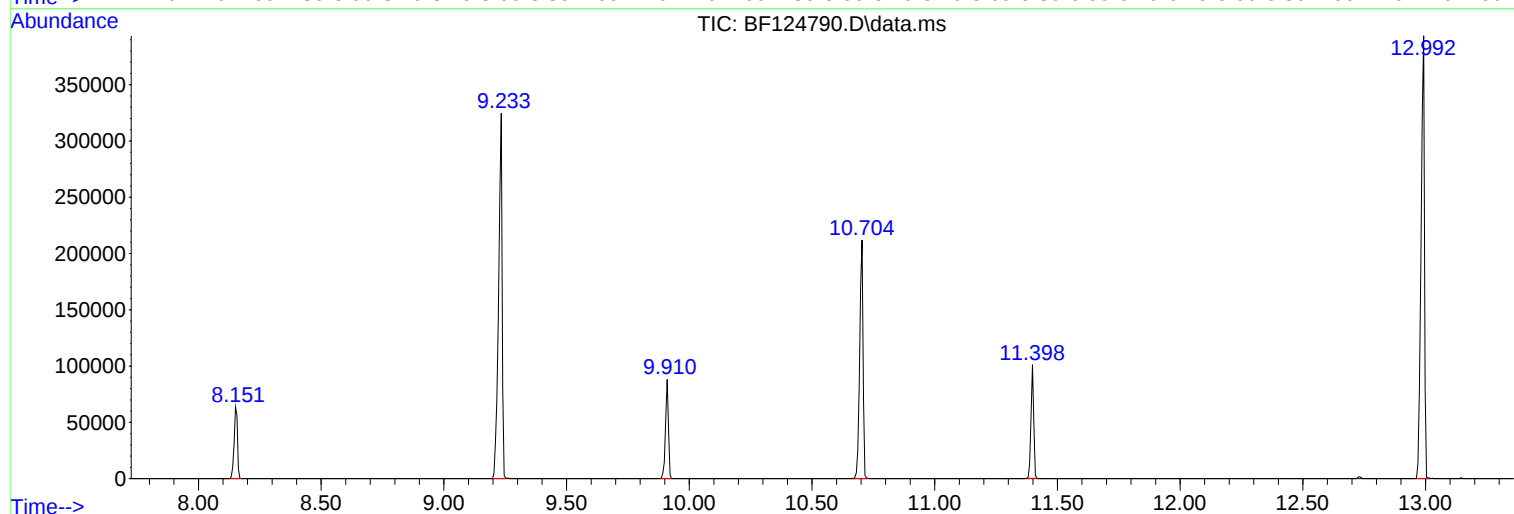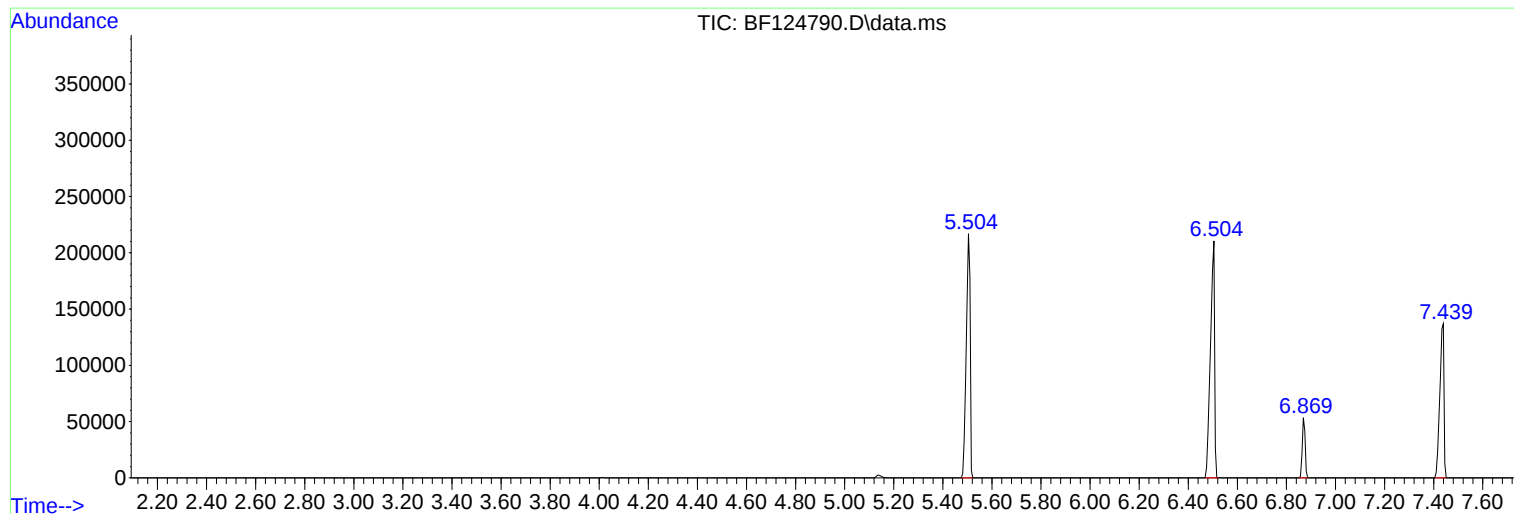

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124790.D
Acq On : 27 Jul 2021 12:26
Operator : JU/CG
Sample : PB137900BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137900BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124790.D
Acq On : 27 Jul 2021 12:26
Operator : JU/CG
Sample : PB137900BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137900BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------