

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
 Data File : BF124798.D
 Acq On : 27 Jul 2021 17:25
 Operator : JU/CG
 Sample : PB137931BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137931BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	516	519	523	rBB	2810	3646	1.21%	0.210%
2	5.504	576	581	584	rBB	217008	238526	78.91%	13.733%
3	6.504	745	751	753	rBV	204485	238699	78.97%	13.742%
4	6.869	810	813	816	rBB	58687	44667	14.78%	2.572%
5	7.434	904	909	912	rBB	137429	159009	52.61%	9.155%
6	8.151	1027	1031	1035	rBB	65363	59586	19.71%	3.431%
7	9.234	1209	1215	1218	rBV	322167	299456	99.07%	17.240%
8	9.910	1325	1330	1333	rBB	82188	66582	22.03%	3.833%
9	10.704	1460	1465	1468	rBV	176284	174183	57.63%	10.028%
10	11.398	1579	1583	1586	rBV	82242	66635	22.05%	3.836%
11	12.986	1848	1853	1856	rBV	311555	302259	100.00%	17.402%
12	14.033	2028	2031	2035	rBV2	58542	48113	15.92%	2.770%
13	15.510	2277	2282	2288	rBB	29220	35580	11.77%	2.048%




Sum of corrected areas: 1736941

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124798.D
Acq On : 27 Jul 2021 17:25
Operator : JU/CG
Sample : PB137931BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137931BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

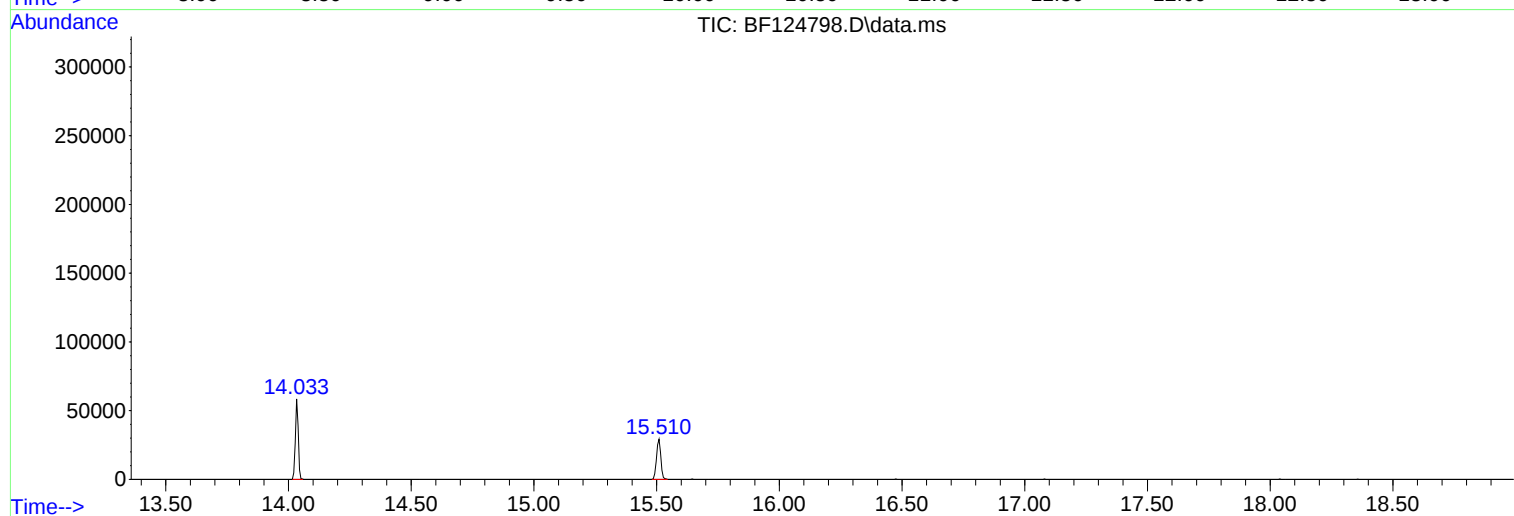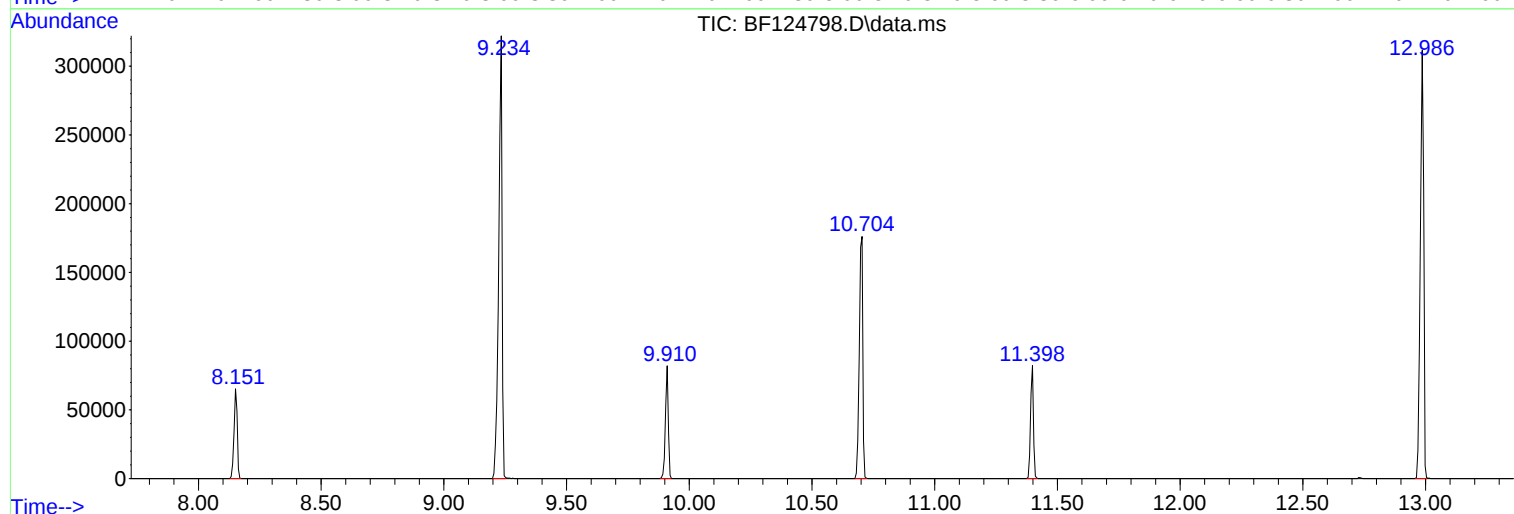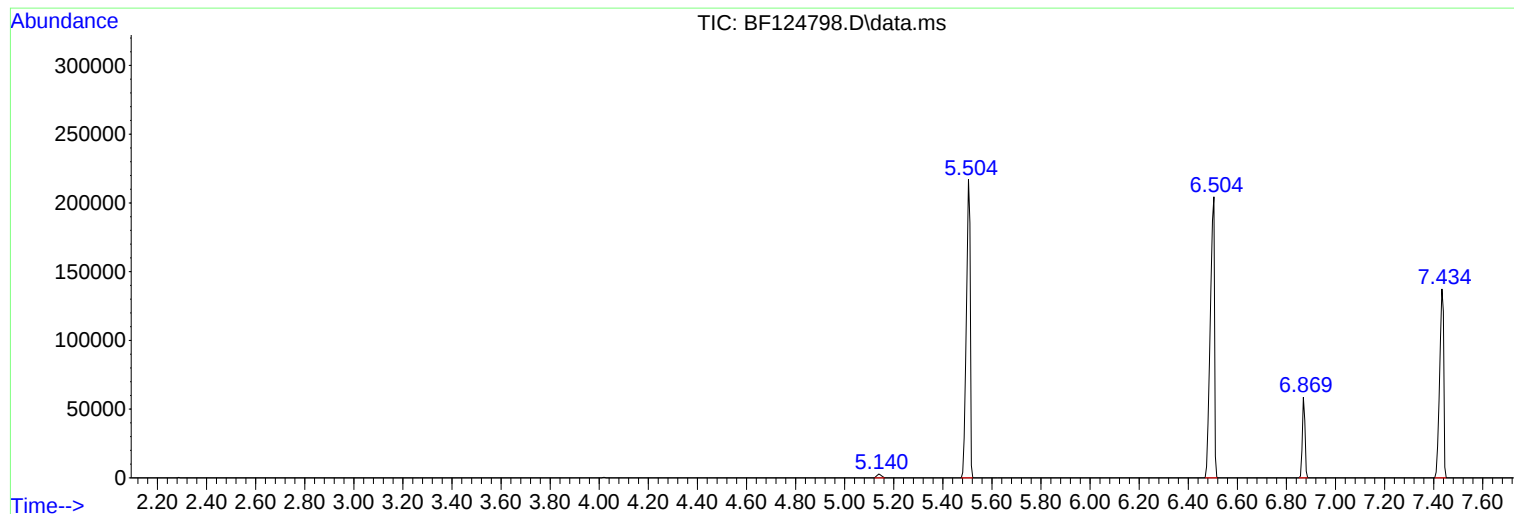

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124798.D
Acq On : 27 Jul 2021 17:25
Operator : JU/CG
Sample : PB137931BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137931BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124798.D
Acq On : 27 Jul 2021 17:25
Operator : JU/CG
Sample : PB137931BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137931BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------