

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
 Data File : BF124814.D
 Acq On : 28 Jul 2021 2:31
 Operator : JU/CG
 Sample : M3183-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-201-RBR-200036

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	573	575	578	rBB	8004	7211	13.76%	2.078%
2	6.487	745	748	750	rBB	12595	8383	16.00%	2.416%
3	6.869	810	813	816	rBB	46855	34892	66.59%	10.056%
4	7.428	905	908	910	rBB	8266	5580	10.65%	1.608%
5	8.151	1028	1031	1035	rBB	53045	46009	87.81%	13.260%
6	9.228	1211	1214	1218	rBB	11712	9671	18.46%	2.787%
7	9.910	1327	1330	1333	rBV	67897	52397	100.00%	15.101%
8	10.692	1461	1463	1466	rBB	5118	3264	6.23%	0.941%
9	11.398	1579	1583	1586	rBV	58432	48289	92.16%	13.917%
10	12.980	1849	1852	1854	rBB	9532	7815	14.91%	2.252%
11	14.033	2028	2031	2035	rBB	40570	33549	64.03%	9.669%
12	14.168	2053	2054	2057	rBV	690	728	1.39%	0.210%
13	14.221	2062	2063	2066	rBV	691	824	1.57%	0.237%
14	14.298	2074	2076	2078	rVB	882	690	1.32%	0.199%
15	14.374	2082	2089	2090	rBV	776	1166	2.23%	0.336%
16	14.439	2099	2100	2102	rBV	1526	1313	2.51%	0.378%
17	14.515	2112	2113	2115	rBV	823	710	1.36%	0.205%
18	14.551	2117	2119	2120	rBV	770	659	1.26%	0.190%
19	14.704	2140	2145	2147	rBV2	1216	1941	3.70%	0.559%
20	14.733	2147	2150	2152	rBV	1012	931	1.78%	0.268%
21	14.810	2161	2163	2165	rBV	641	739	1.41%	0.213%
22	14.909	2177	2180	2183	rVB2	896	718	1.37%	0.207%
23	14.939	2183	2185	2186	rBV2	1263	722	1.38%	0.208%
24	14.968	2186	2190	2192	rVB2	680	853	1.63%	0.246%
25	15.039	2195	2202	2204	rVB3	838	1425	2.72%	0.411%
26	15.068	2204	2207	2210	rBV	1609	1780	3.40%	0.513%
27	15.139	2217	2219	2220	rBV	821	780	1.49%	0.225%
28	15.186	2226	2227	2229	rBV2	819	721	1.38%	0.208%
29	15.257	2235	2239	2240	rBV3	892	930	1.77%	0.268%
30	15.274	2240	2242	2244	rVB	854	860	1.64%	0.248%
31	15.292	2244	2245	2248	rBV	1185	731	1.40%	0.211%
32	15.368	2254	2258	2259	rVB2	1118	708	1.35%	0.204%
33	15.404	2262	2264	2267	rBV	882	862	1.65%	0.248%
34	15.451	2267	2272	2273	rBV2	938	1274	2.43%	0.367%
35	15.462	2273	2274	2277	rVB2	964	799	1.52%	0.230%
36	15.509	2277	2282	2288	rBV	24500	30184	57.61%	8.699%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
 Data File : BF124814.D
 Acq On : 28 Jul 2021 2:31
 Operator : JU/CG
 Sample : M3183-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-201-RBR-200036

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.586	2293	2295	2298	rVB2	1070	1124	2.15%	0.324%
38	15.627	2298	2302	2305	rVB3	860	1489	2.84%	0.429%
39	15.657	2305	2307	2310	rBV	1071	1085	2.07%	0.313%
40	15.709	2314	2316	2317	rBV2	985	849	1.62%	0.245%
41	15.745	2320	2322	2323	rBV	1096	722	1.38%	0.208%
42	15.786	2326	2329	2330	rBV	1046	916	1.75%	0.264%
43	15.845	2335	2339	2343	rBV2	1351	1990	3.80%	0.574%
44	15.874	2343	2344	2347	rVB	758	717	1.37%	0.207%
45	16.033	2368	2371	2372	rBV	899	709	1.35%	0.204%
46	16.151	2388	2391	2392	rBV	929	748	1.43%	0.216%
47	16.168	2392	2394	2396	rVB	817	698	1.33%	0.201%
48	16.192	2396	2398	2399	rBV	1045	779	1.49%	0.225%
49	16.221	2399	2403	2406	rVV3	1629	2240	4.28%	0.646%
50	16.374	2427	2429	2431	rVB	1732	1076	2.05%	0.310%
51	16.415	2434	2436	2438	rVB	802	747	1.43%	0.215%
52	16.445	2438	2441	2443	rBV2	1014	1021	1.95%	0.294%
53	16.515	2450	2453	2455	rBV3	1077	1059	2.02%	0.305%
54	16.551	2458	2459	2461	rVB	1466	649	1.24%	0.187%
55	16.580	2461	2464	2465	rBV	951	848	1.62%	0.244%
56	16.592	2465	2466	2470	rVB	1526	1796	3.43%	0.518%
57	16.621	2470	2471	2473	rBV	1130	1020	1.95%	0.294%
58	16.903	2516	2519	2520	rVB2	1047	875	1.67%	0.252%
59	16.927	2520	2523	2524	rBV	1236	970	1.85%	0.280%
60	17.086	2547	2550	2551	rVB	935	919	1.75%	0.265%
61	17.151	2559	2561	2563	rBV	731	666	1.27%	0.192%
62	17.245	2576	2577	2580	rVB	978	688	1.31%	0.198%
63	17.280	2580	2583	2586	rVB	538	668	1.27%	0.193%
64	17.315	2586	2589	2591	rVB	945	698	1.33%	0.201%
65	17.403	2602	2604	2607	rVB	1100	1018	1.94%	0.293%
66	17.456	2610	2613	2616	rVB	1088	1153	2.20%	0.332%
67	17.486	2616	2618	2619	rBV	757	658	1.26%	0.190%
68	17.686	2649	2652	2653	rBV	838	855	1.63%	0.246%
69	17.792	2667	2670	2672	rBV	825	1057	2.02%	0.305%
70	17.821	2674	2675	2678	rBV	719	761	1.45%	0.219%
71	17.892	2686	2687	2690	rBV	789	1067	2.04%	0.308%
72	17.927	2692	2693	2696	rBV	703	830	1.58%	0.239%
73	18.227	2743	2744	2747	rVB	766	651	1.24%	0.188%
74	18.509	2790	2792	2795	rVB2	1018	1046	2.00%	0.301%

Sum of corrected areas: 346970


Instrument :
BNA_F
ClientSampleId :
VNJ-201-RBR-200036

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124814.D
Acq On : 28 Jul 2021 2:31
Operator : JU/CG
Sample : M3183-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-201-RBR-200036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

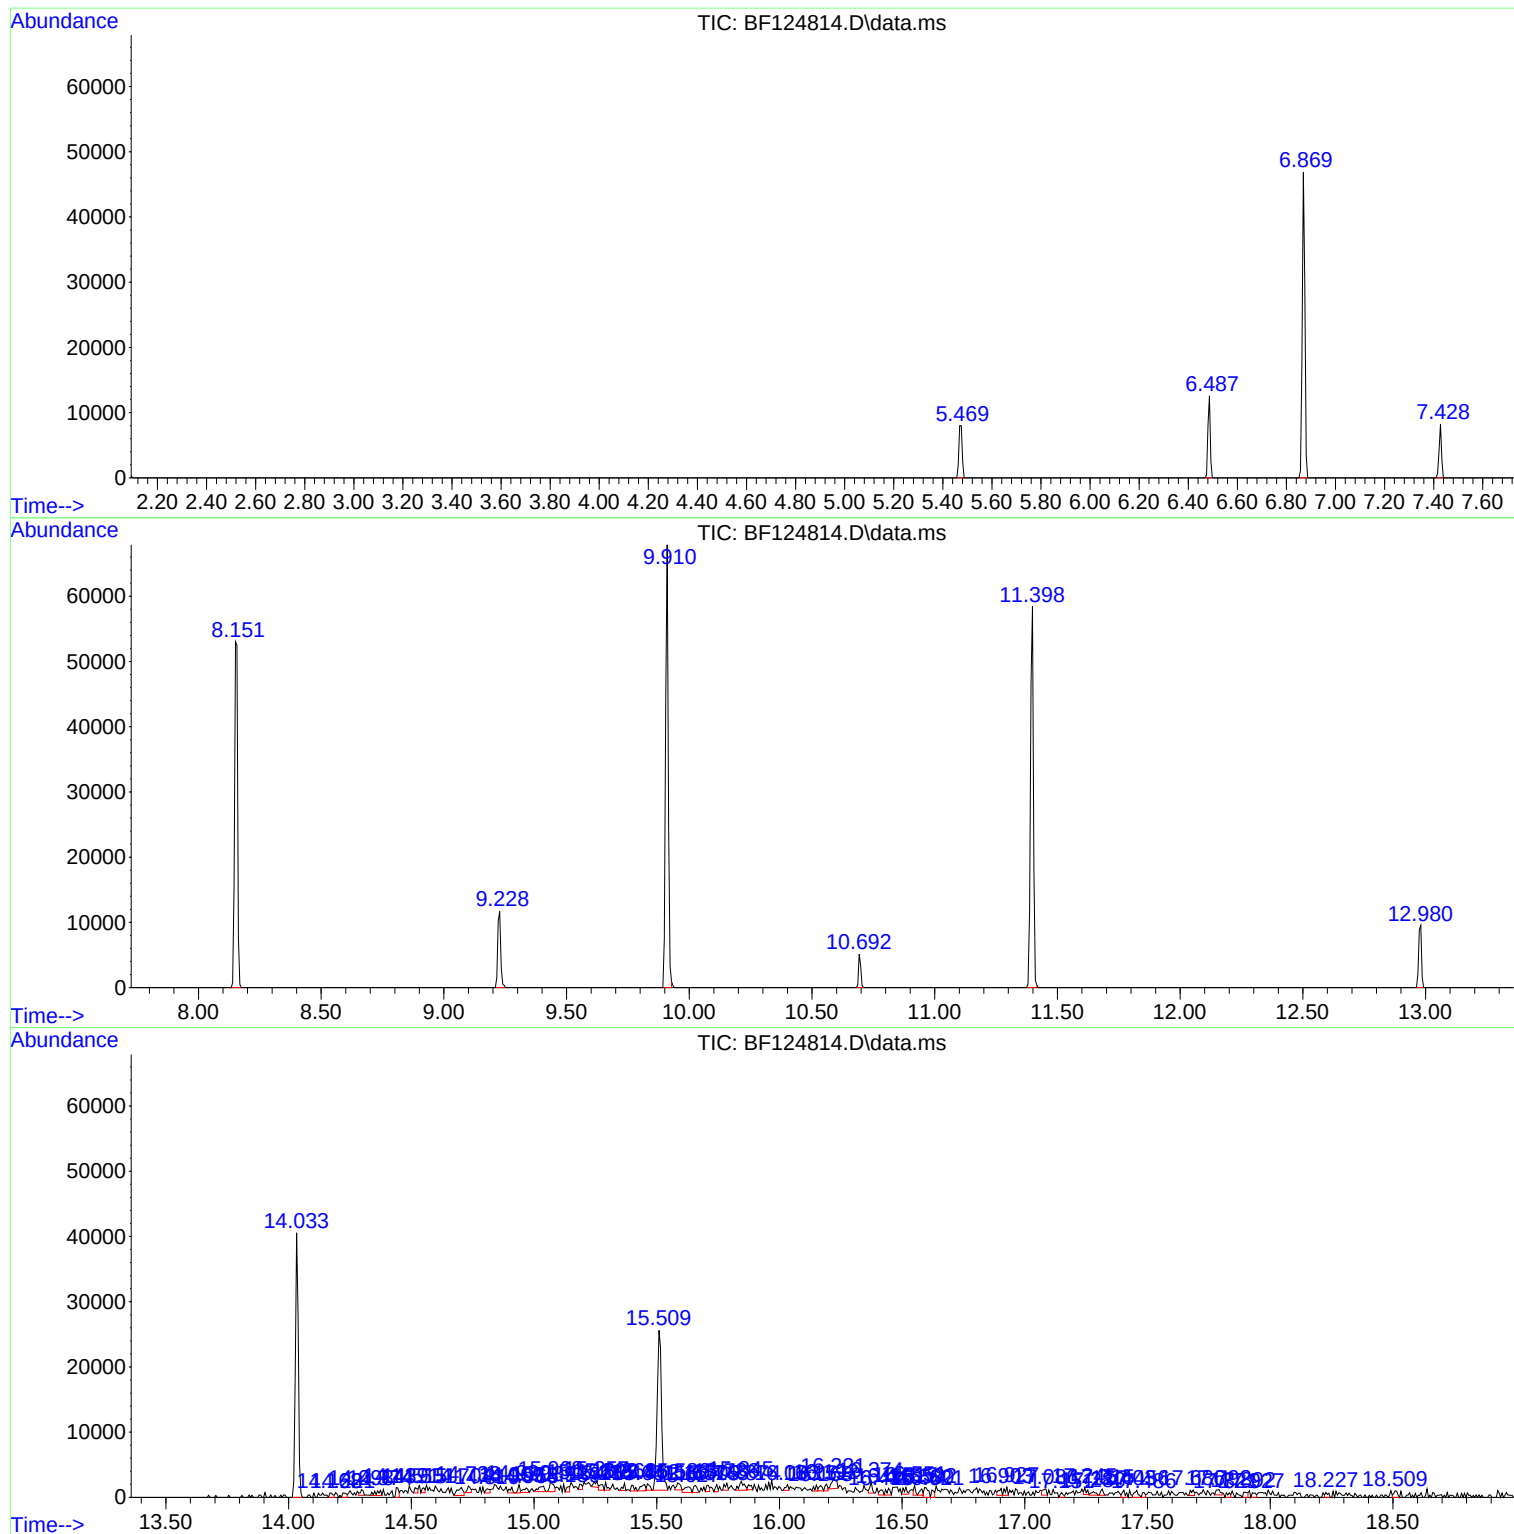

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124814.D
Acq On : 28 Jul 2021 2:31
Operator : JU/CG
Sample : M3183-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-201-RBR-200036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
Data File : BF124814.D
Acq On : 28 Jul 2021 2:31
Operator : JU/CG
Sample : M3183-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-201-RBR-200036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
