


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072721\
 Data File : BF124784.D
 Acq On : 27 Jul 2021 9:08
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

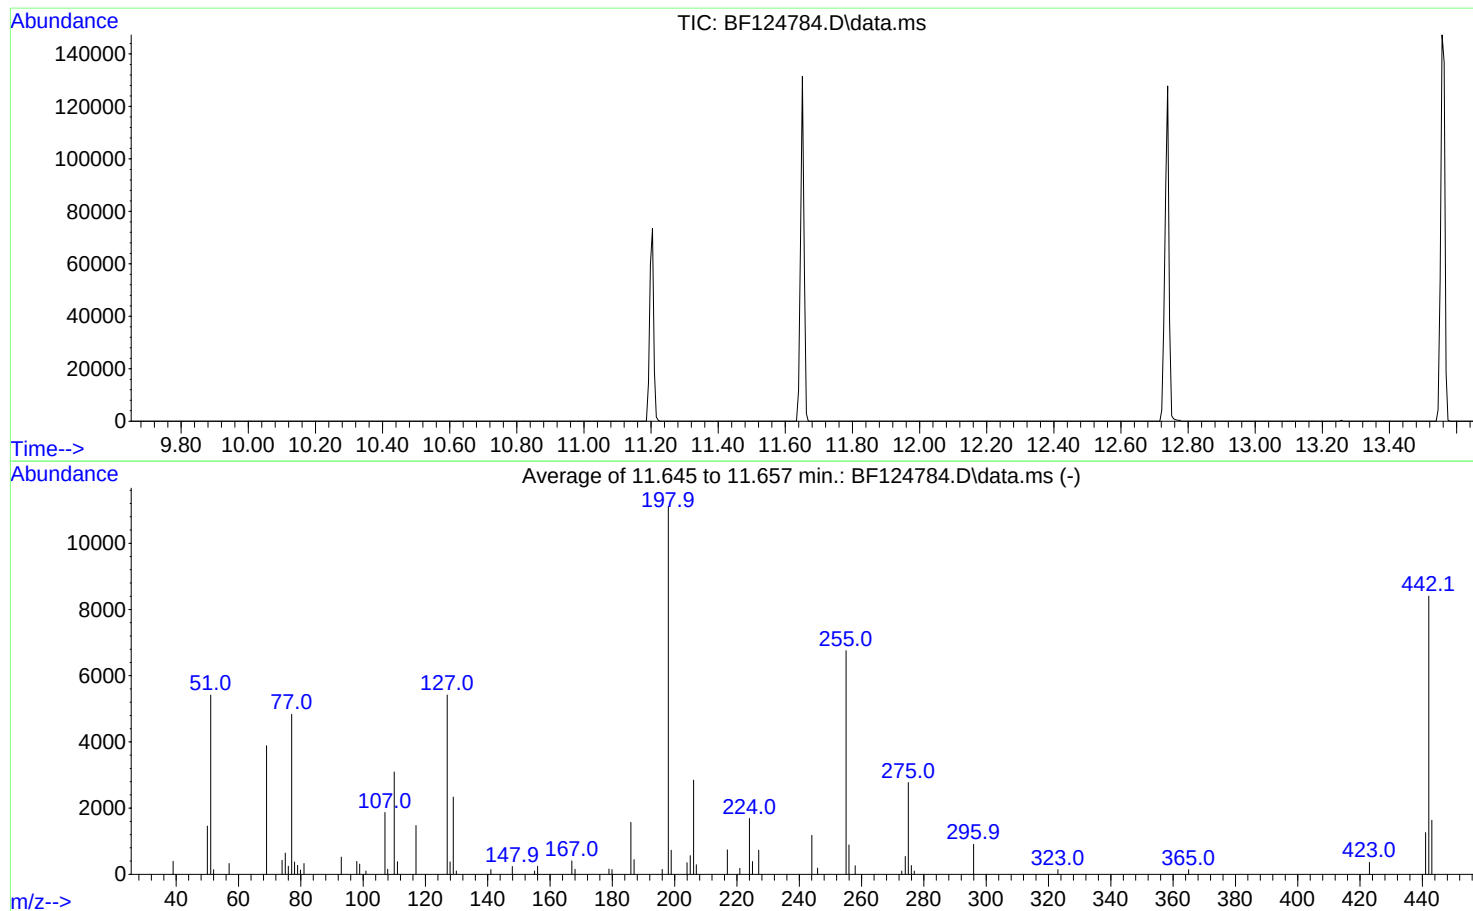

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	5413	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.0	3888	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	5418	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11110	PASS
199	198	5	9	6.6	729	PASS
275	198	10	60	25.0	2774	PASS
365	198	1	100	1.3	142	PASS
441	198	0.01	100	11.3	1260	PASS
442	442	50	100	100.0	8402	PASS
443	442	15	24	19.4	1632	PASS