

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
 Data File : BF129368.D
 Acq On : 27 Jul 2022 10:16
 Operator : CG\JU
 Sample : PB146469BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146469BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	543	548	551	rBV	5303341	5018911	53.05%	10.727%
2	6.510	712	718	721	rBV	4895053	5018057	53.04%	10.725%
3	6.881	777	781	785	rBV	1950806	1513233	16.00%	3.234%
4	7.445	872	877	880	rBV	3461303	3343282	35.34%	7.146%
5	8.163	995	999	1003	rBV	2298360	2033861	21.50%	4.347%
6	9.239	1176	1182	1186	rBV	6082027	6118487	64.67%	13.078%
7	9.922	1293	1298	1302	rBV	2760047	2334517	24.68%	4.990%
8	10.716	1426	1433	1436	rBV	5434340	5457038	57.68%	11.664%
9	11.416	1547	1552	1555	rBV	2684402	2376522	25.12%	5.080%
10	13.010	1817	1823	1826	rBV	8766120	9460548	100.00%	20.221%
11	14.057	1997	2001	2005	rBV	2293478	2145966	22.68%	4.587%
12	15.551	2249	2255	2269	rBV	1529647	1965861	20.78%	4.202%




Sum of corrected areas: 46786283

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129368.D
Acq On : 27 Jul 2022 10:16
Operator : CG\JU
Sample : PB146469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146469BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

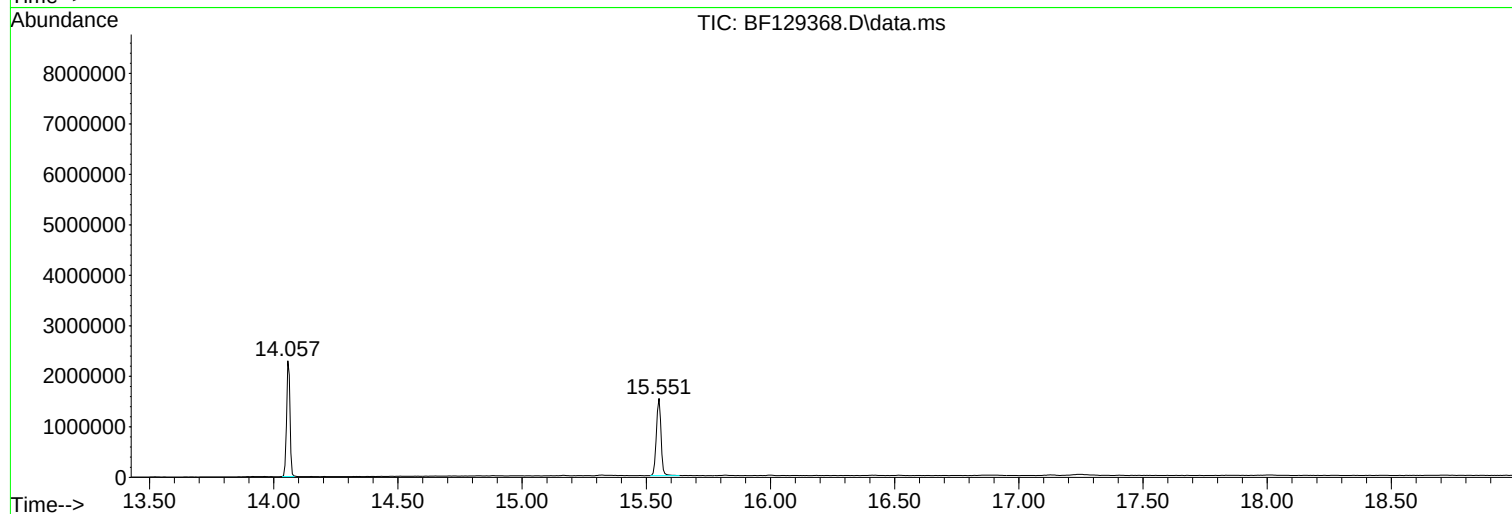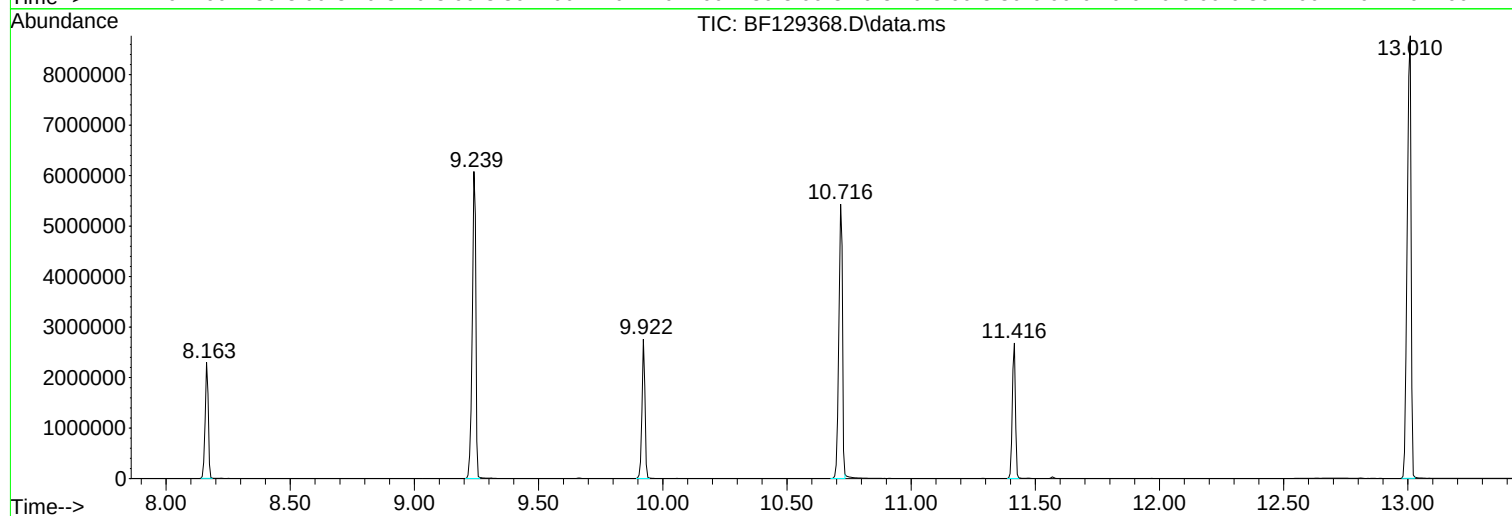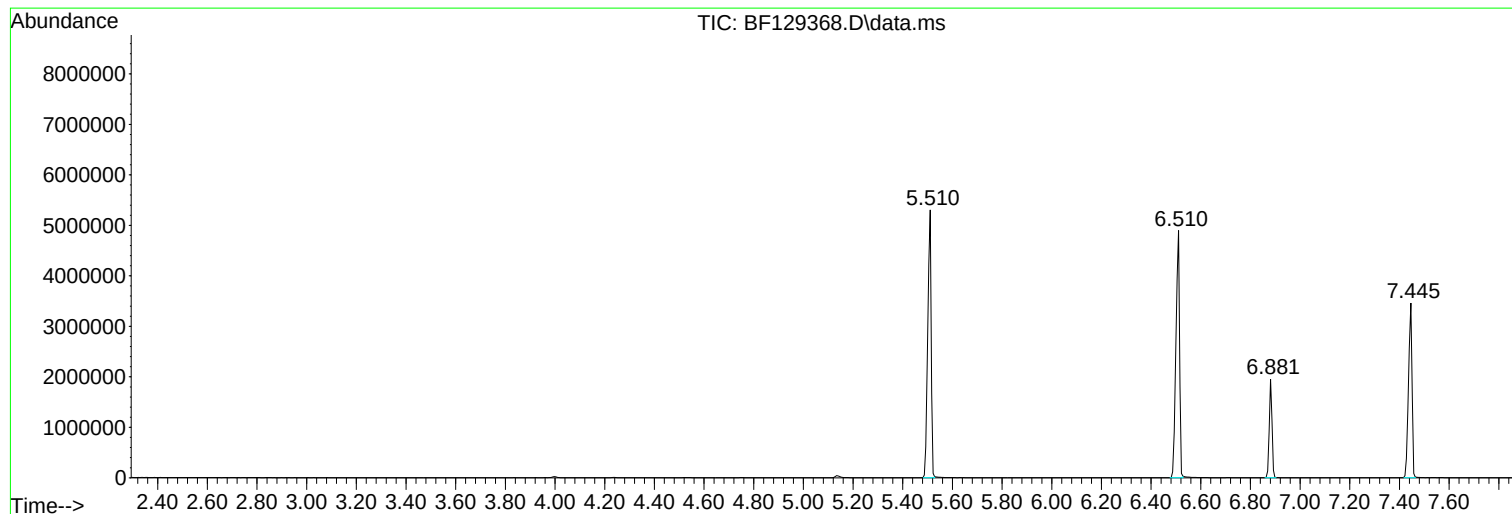

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129368.D
Acq On : 27 Jul 2022 10:16
Operator : CG\JU
Sample : PB146469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146469BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129368.D
Acq On : 27 Jul 2022 10:16
Operator : CG\JU
Sample : PB146469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146469BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------