

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
 Data File : BF129389.D
 Acq On : 27 Jul 2022 22:10
 Operator : CG\JU
 Sample : N3887-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	479	481	489	rBV	76452	94779	1.09%	0.215%
2	5.510	543	548	551	rBV	4173315	3667458	42.15%	8.336%
3	5.675	571	576	582	rVB	105276	93971	1.08%	0.214%
4	5.934	617	620	626	rVB	103585	87405	1.00%	0.199%
5	6.216	665	668	671	rBV	119040	96068	1.10%	0.218%
6	6.510	714	718	725	rBV	2486990	2346371	26.97%	5.333%
7	6.881	777	781	785	rBV	1811248	1503793	17.28%	3.418%
8	7.075	808	814	827	rVB2	100068	161014	1.85%	0.366%
9	7.451	870	878	881	rBV	4760044	5214562	59.93%	11.853%
10	8.163	994	999	1003	rBV	2194500	2004231	23.04%	4.556%
11	9.245	1176	1183	1186	rBV	8917958	8700802	100.00%	19.777%
12	9.922	1292	1298	1302	rBV	2545215	2215226	25.46%	5.035%
13	10.722	1426	1434	1437	rBV	5236108	5582239	64.16%	12.689%
14	11.416	1548	1552	1555	rBV	2389666	2063444	23.72%	4.690%
15	13.004	1817	1822	1825	rBV	7714660	7408444	85.15%	16.840%
16	13.904	1970	1975	1982	rBV4	59509	125019	1.44%	0.284%
17	14.057	1997	2001	2005	rBV	1639060	1438304	16.53%	3.269%
18	15.551	2250	2255	2266	rVB	932039	1190793	13.69%	2.707%




Sum of corrected areas: 43993923

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129389.D
Acq On : 27 Jul 2022 22:10
Operator : CG\JU
Sample : N3887-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

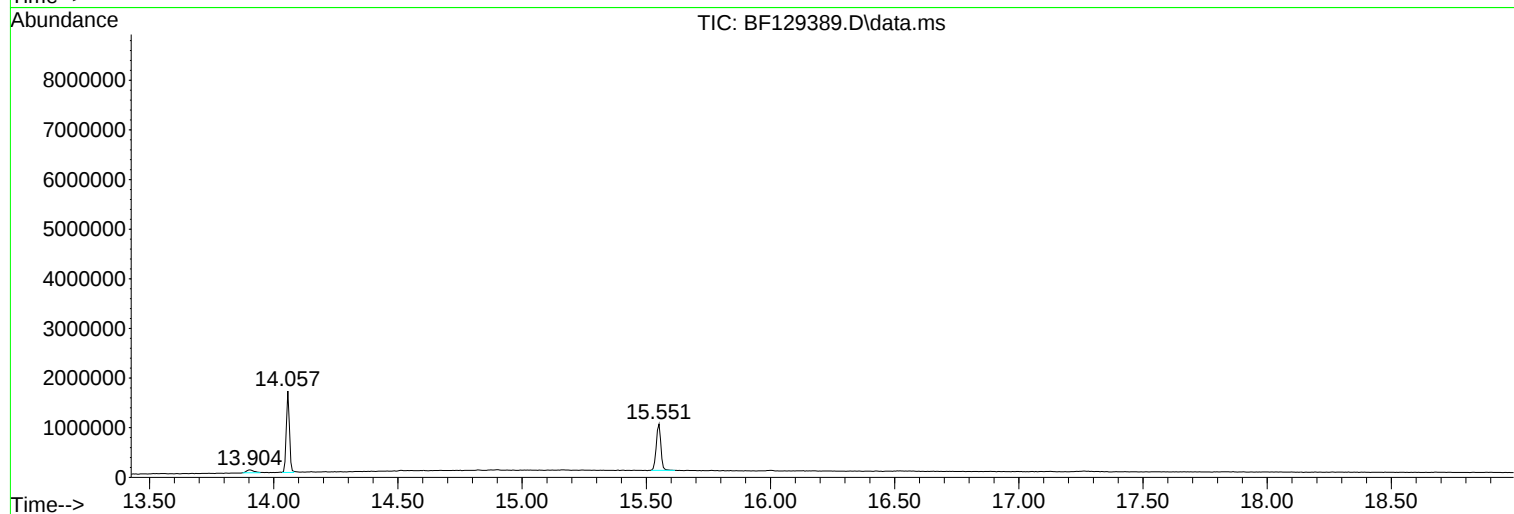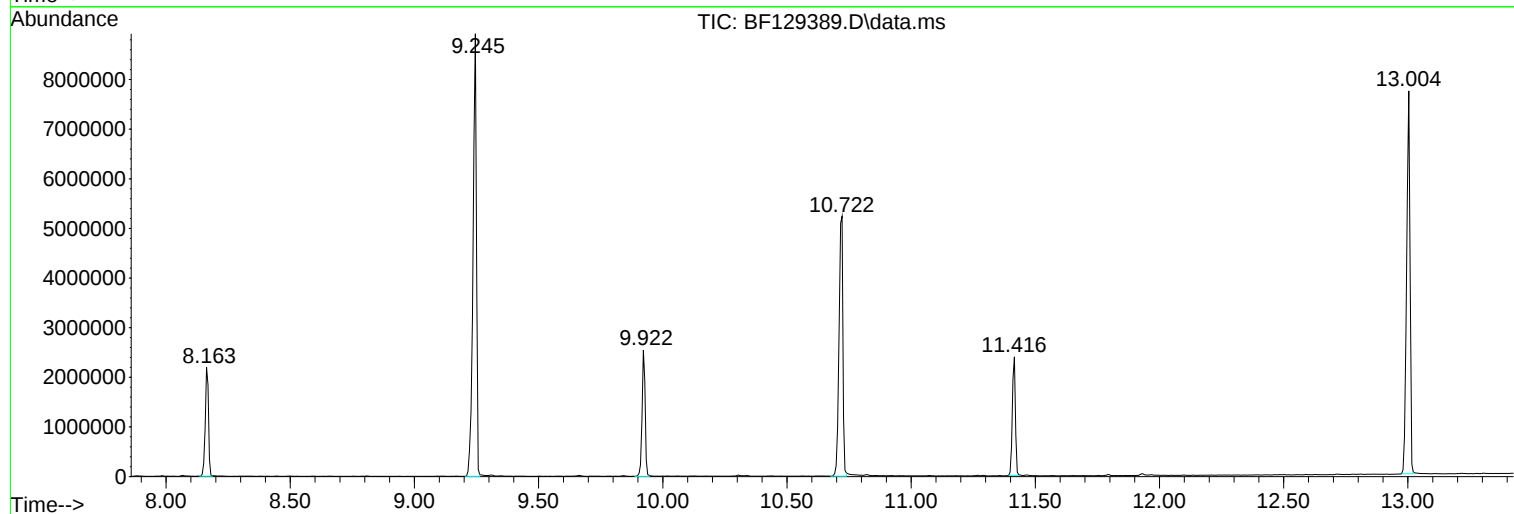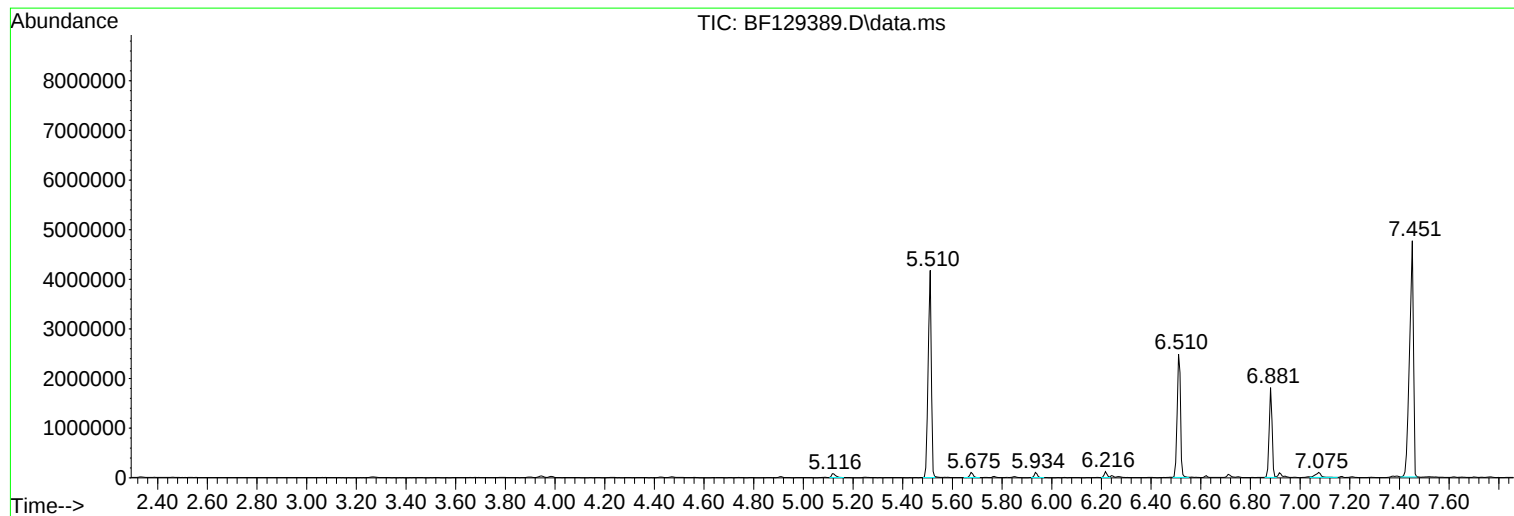

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129389.D
Acq On : 27 Jul 2022 22:10
Operator : CG\JU
Sample : N3887-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129389.D
Acq On : 27 Jul 2022 22:10
Operator : CG\JU
Sample : N3887-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------