

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
 Data File : BF129393.D
 Acq On : 28 Jul 2022 00:21
 Operator : CG\JU
 Sample : N3887-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	544	548	552	rBV	4151125	3899592	47.44%	9.520%
2	6.516	714	719	722	rBV	2922997	2485710	30.24%	6.068%
3	6.881	777	781	785	rBV	1855213	1516088	18.44%	3.701%
4	7.451	869	878	881	rBV	4548665	4971089	60.47%	12.136%
5	8.163	995	999	1003	rBV	2229161	2009567	24.44%	4.906%
6	9.245	1176	1183	1186	rBV	8431336	8220868	100.00%	20.070%
7	9.922	1292	1298	1302	rBV	2491919	2172094	26.42%	5.303%
8	10.304	1360	1363	1366	rBV	163418	119460	1.45%	0.292%
9	10.722	1427	1434	1437	rBV	5133686	5148989	62.63%	12.570%
10	11.416	1548	1552	1555	rBV	2198017	1931933	23.50%	4.716%
11	11.933	1637	1640	1644	rBV	120967	125112	1.52%	0.305%
12	13.004	1817	1822	1825	rBV	6365608	5831849	70.94%	14.237%
13	13.904	1972	1975	1980	rBV2	120421	162394	1.98%	0.396%
14	14.057	1998	2001	2005	rBV	1366450	1204434	14.65%	2.940%
15	15.551	2250	2255	2264	rVB	914327	1162745	14.14%	2.839%




Sum of corrected areas: 40961924

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129393.D
Acq On : 28 Jul 2022 00:21
Operator : CG\JU
Sample : N3887-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

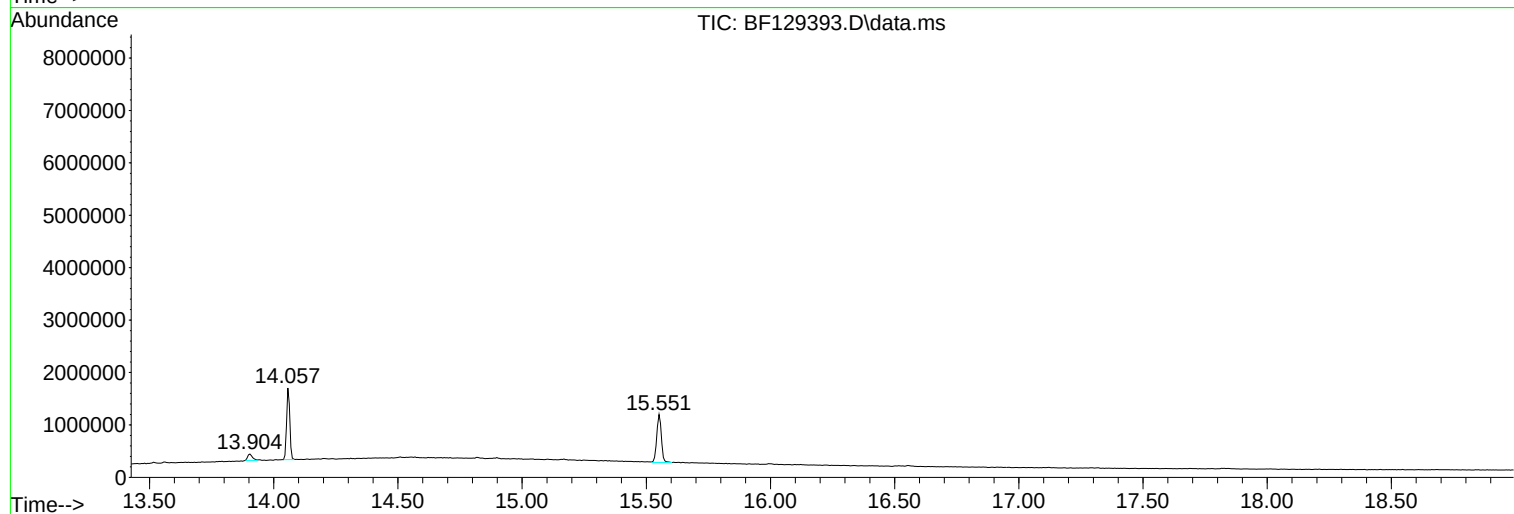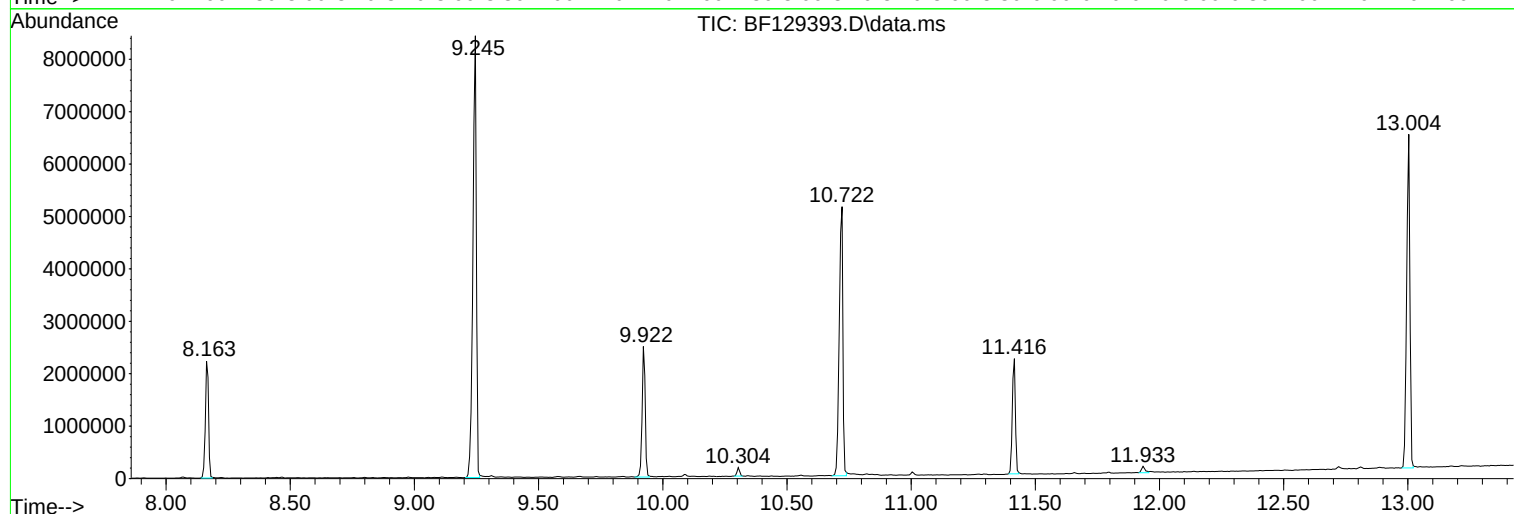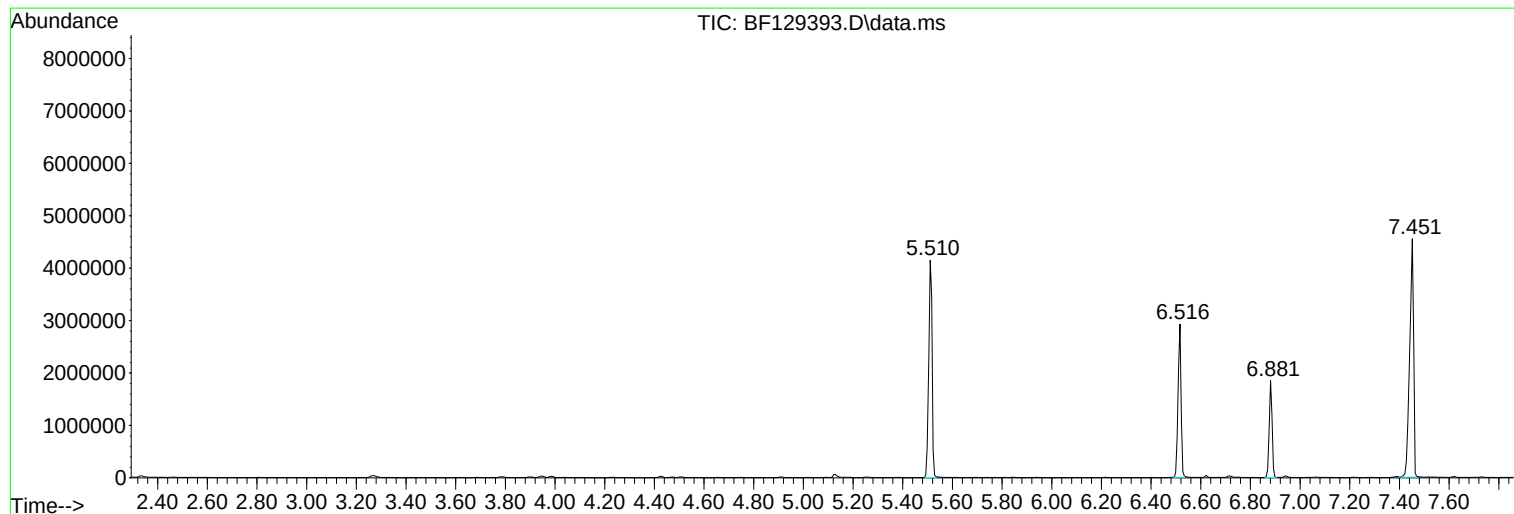

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129393.D
Acq On : 28 Jul 2022 00:21
Operator : CG\JU
Sample : N3887-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-10










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 9-Tricosene, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.904	2.70 ng	162394	Chrysene-d12	14.057

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		9-Tricosene, (Z)-	322	C23H46	027519-02-4	94
2		n-Nonadecanol-1	284	C19H40O	001454-84-8	93
3		Behenic alcohol	326	C22H46O	000661-19-8	91
4		Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	91
5		1-Heneicosanol	312	C21H44O	015594-90-8	91

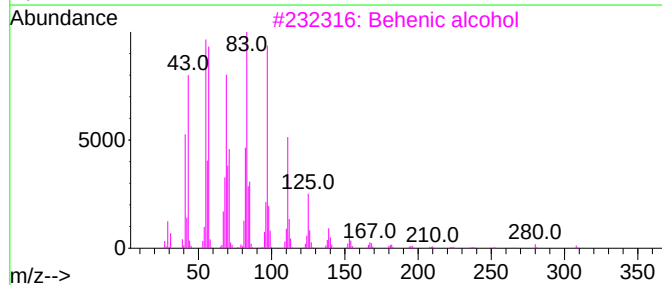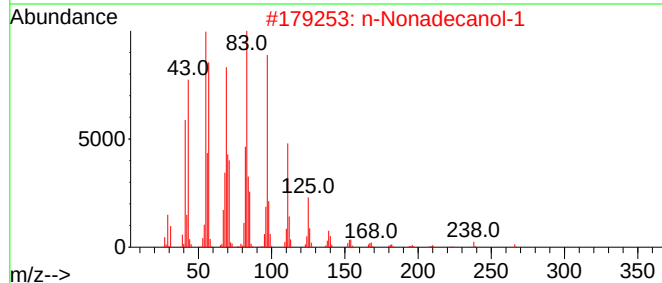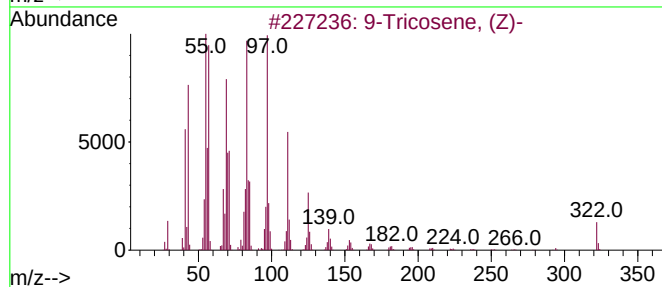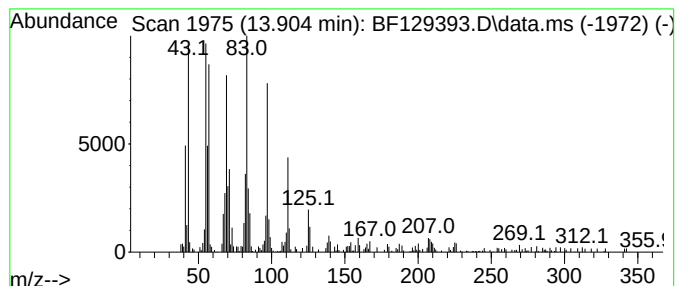

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129393.D
Acq On : 28 Jul 2022 00:21
Operator : CG\JU
Sample : N3887-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
9-Tricosene, (Z)-	13.904	2.7	ng	162394	5	14.057	1204430	20.0