


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
 Data File : BF129366.D
 Acq On : 27 Jul 2022 09:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 17:24:17 2022

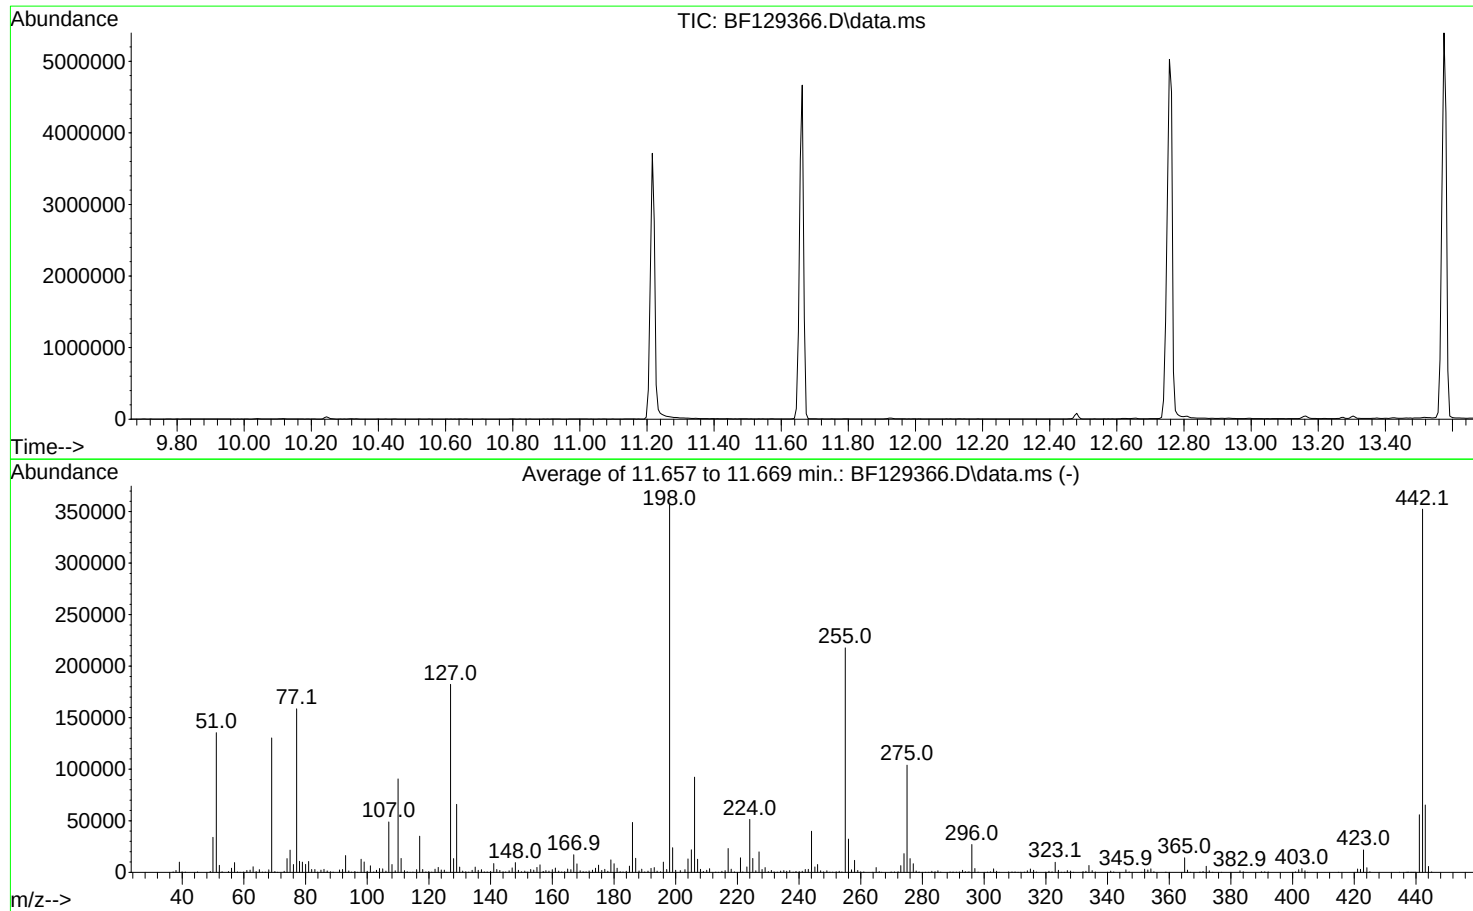




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	135560	PASS
68	69	0.00	2	1.9	2464	PASS
69	198	0.00	100	36.5	130317	PASS
70	69	0.00	2	0.5	675	PASS
127	198	10	80	51.1	182400	PASS
197	198	0.00	2	0.8	2781	PASS
198	198	100	100	100.0	356971	PASS
199	198	5	9	6.7	23904	PASS
275	198	10	60	29.1	103952	PASS
365	198	1	100	4.0	14104	PASS
441	198	0.01	100	15.6	55784	PASS
442	442	50	100	100.0	352341	PASS
443	442	15	24	18.6	65360	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
 Data File : BF129366.D
 Acq On : 27 Jul 2022 09:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 28 06:00:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

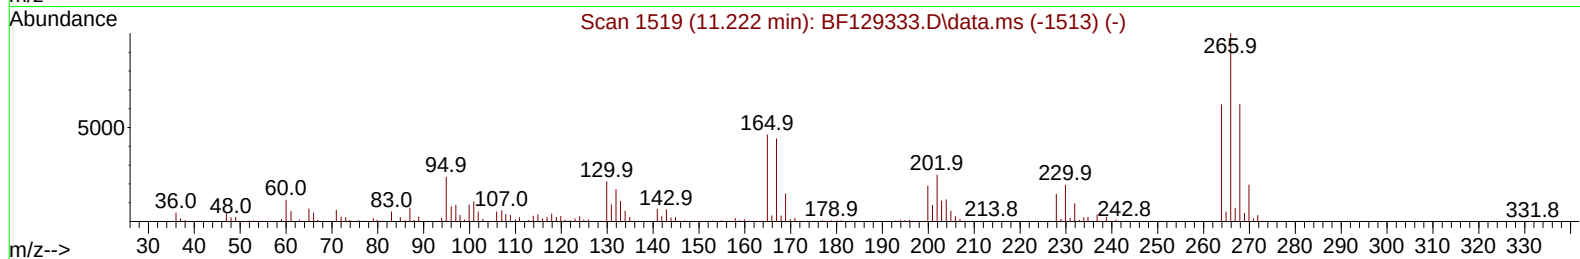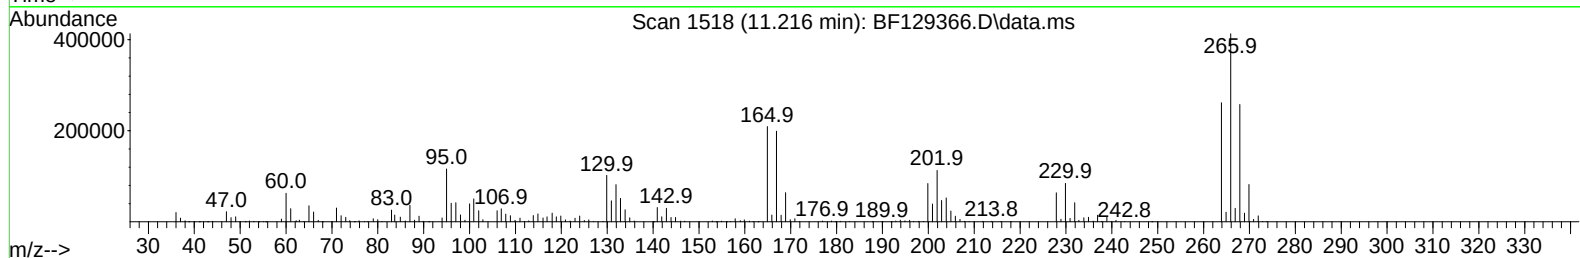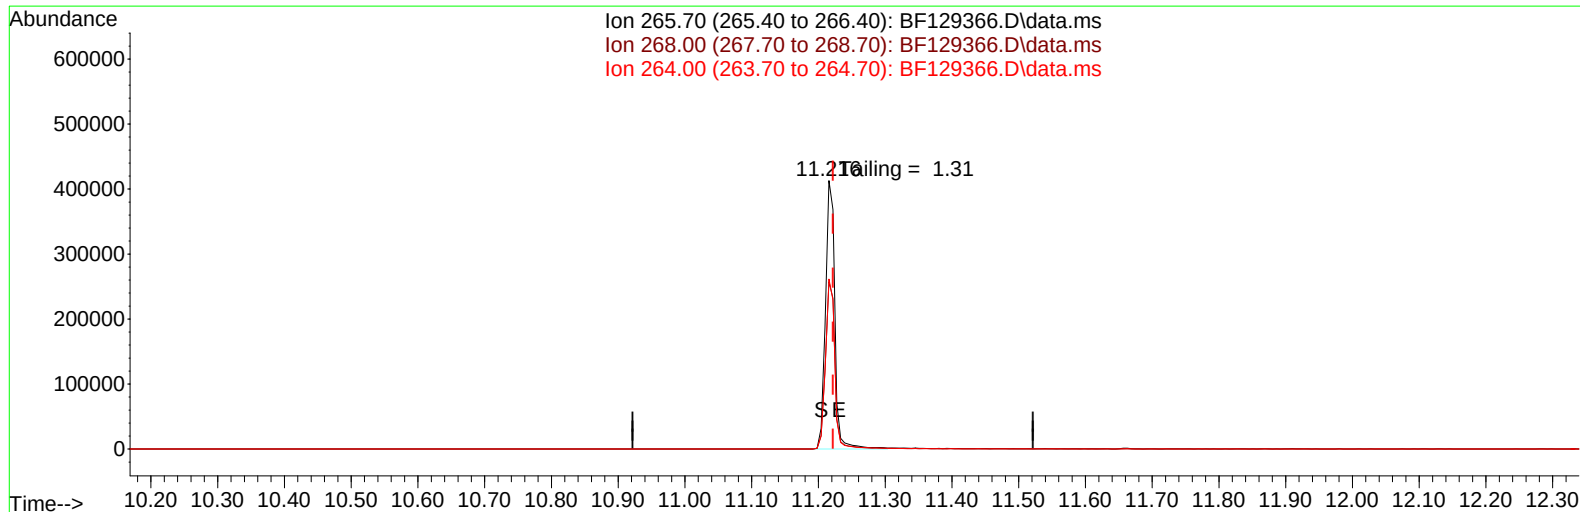

TIC: BF129366.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 563578.59 ng




response 403505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.37
264.00	61.80	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072722\
Data File : BF129366.D
Acq On : 27 Jul 2022 09:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 28 06:00:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

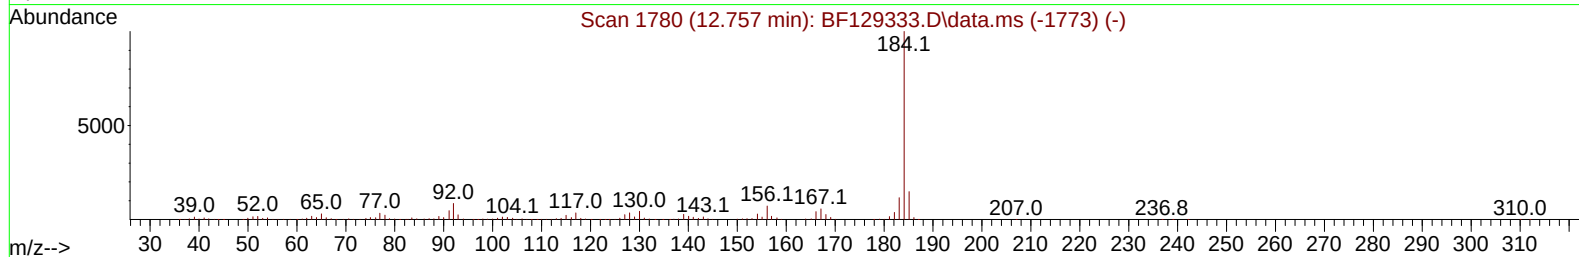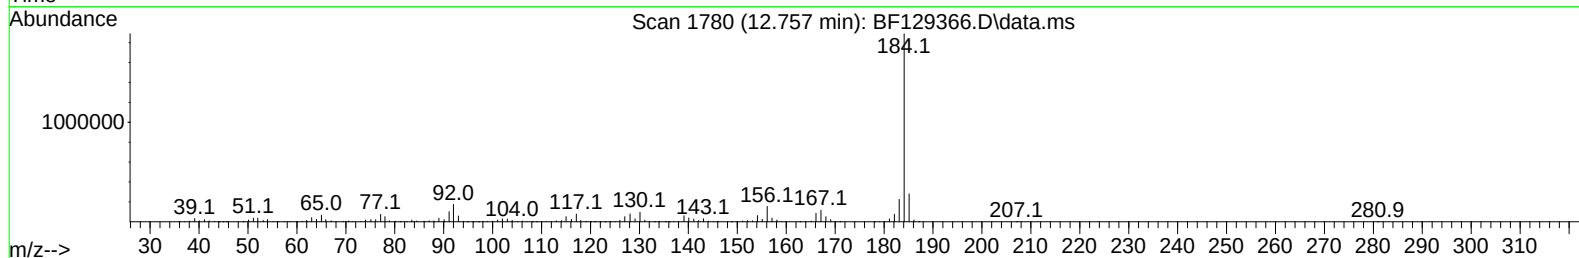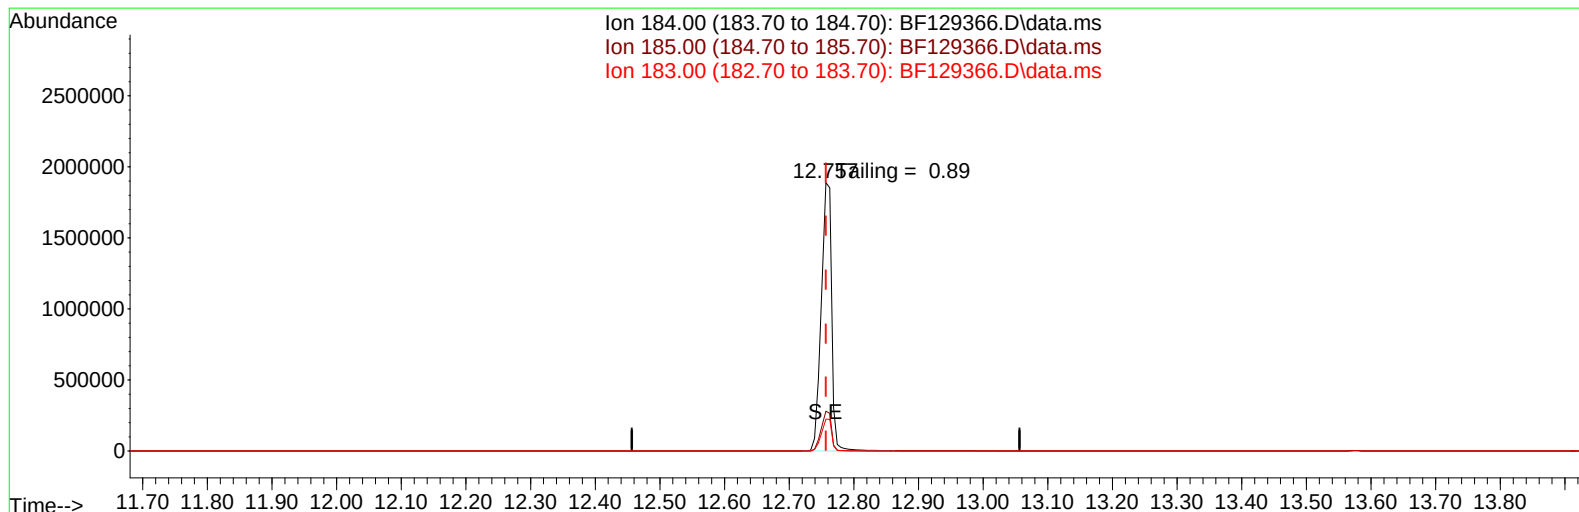

TIC: BF129366.D\data.ms

(77) Benzidine

12.757min (+ 0.000) 231293.31 ng

response 2132636

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.83
183.00	11.60	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/27/2022	BNA_F	<u>BF129366.D</u>
Compound Name	Response	Retention Time
DDT	963568	13.574
DDD	8148	13.304
DDE	898	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9046	972614	0.93

Instrument :
BNA_F
ClientSampleId :
DFTPP