
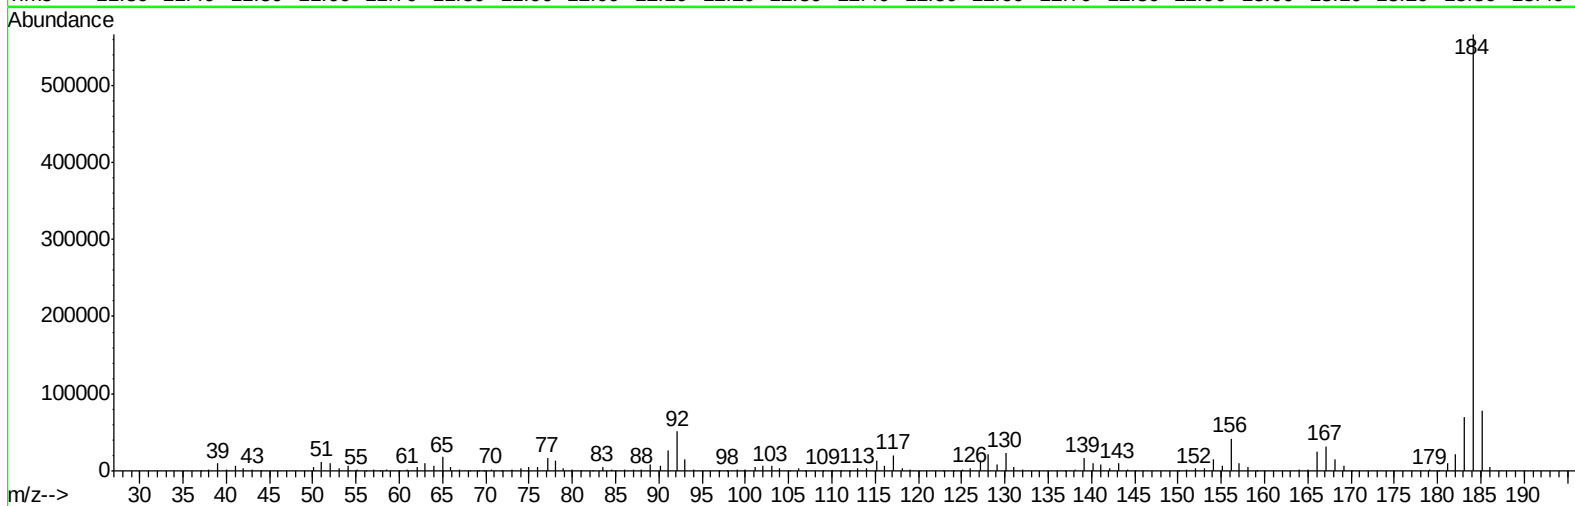


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072817\
Data File : BF097141.D
Acq On : 28 Jul 2017 8:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 06:04:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

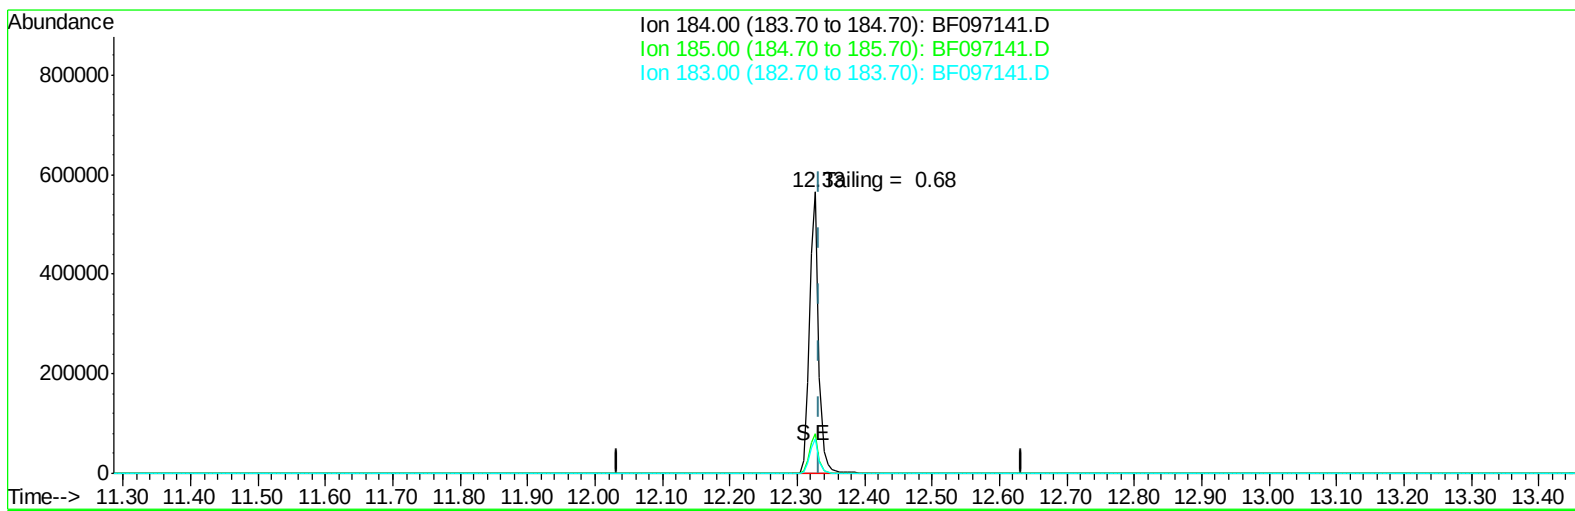

TIC: BF097141.D

(76) Benzidine



12.327min (-0.006) 3026.79ng

response 532904

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.90#
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072817\
Data File : BF097141.D
Acq On : 28 Jul 2017 8:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 06:04:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

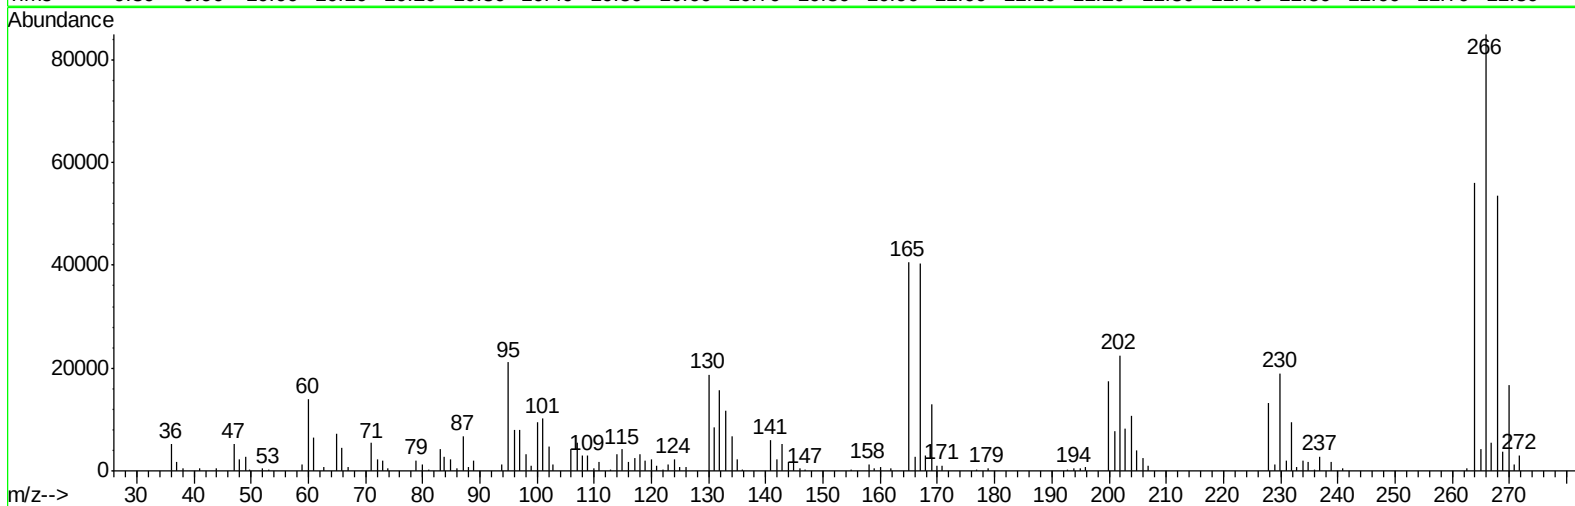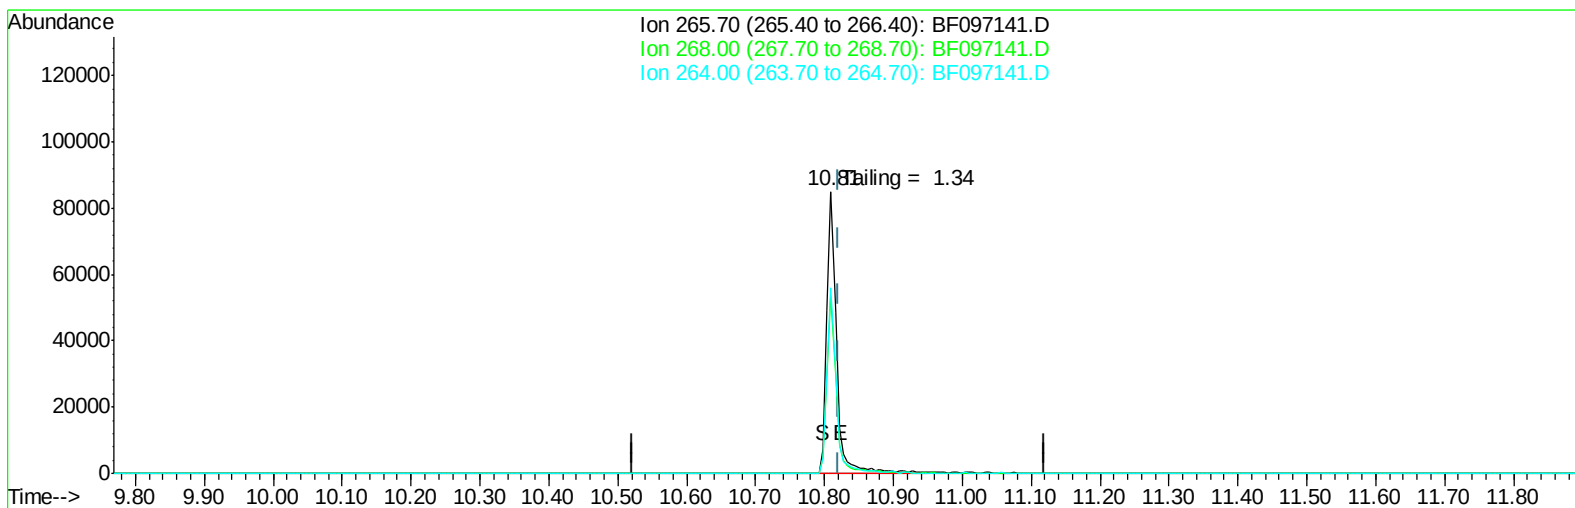

TIC: BF097141.D

(69) Pentachlorophenol (C)

10.810min (-0.011) 11042.32ng

response 80224

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.95
264.00	64.60	65.91
0.00	0.00	0.00