

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072817\
 Data File : BF097173.D
 Acq On : 29 Jul 2017 00:14
 Operator : SJ/JU
 Sample : I4456-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUP

Quant Time: Jul 29 01:33:57 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.49	152	115887	20.00	ng	-0.01
21) Naphthalene-d8	7.77	136	439355	20.00	ng	-0.02
38) Acenaphthene-d10	9.51	164	157800	20.00	ng	-0.02
63) Phenanthrene-d10	10.99	188	211754	20.00	ng	-0.02
75) Chrysene-d12	13.61	240	198252	20.00	ng	-0.02
86) Perylene-d12	14.96	264	162847	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.09	112	769031	100.04	ng	0.00
7) Phenol-d6	6.15	99	958668	109.24	ng	-0.02
23) Nitrobenzene-d5	7.06	82	517022	69.03	ng	-0.02
41) 2,4,6-Tribromophenol	10.30	330	113551	91.08	ng	-0.02
44) 2-Fluorobiphenyl	8.85	172	697776	75.04	ng	-0.02
78) Terphenyl-d14	12.57	244	408944	42.06	ng	-0.02
Target Compounds						
10) Phenol	6.16	94	26651	2.560	ng	96
49) Dimethylphthalate	9.25	163	165725	13.830	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072817\
Data File : BF097173.D
Acq On : 29 Jul 2017 00:14
Operator : SJ/JU
Sample : I4456-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP

Quant Time: Jul 29 01:33:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

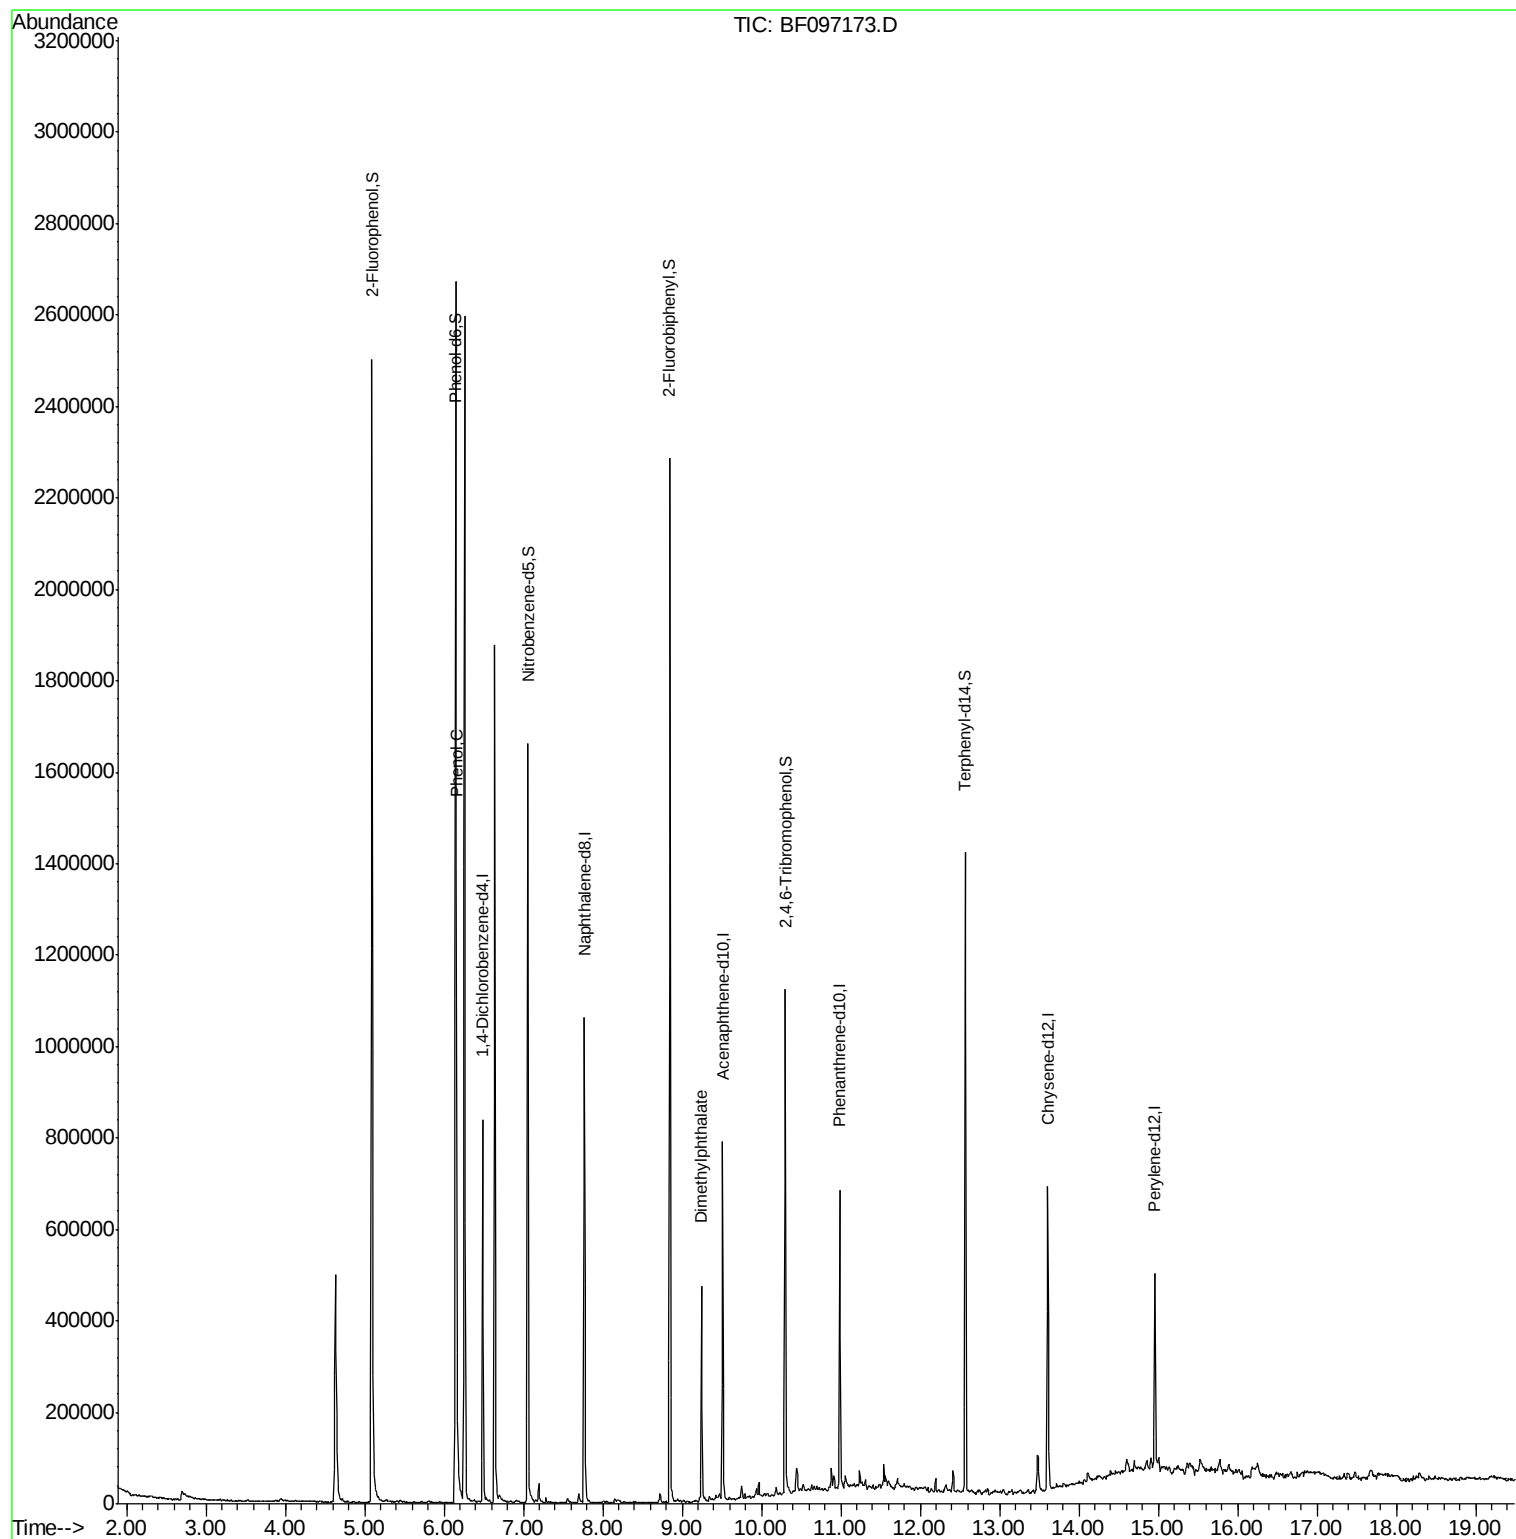




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.49 min Scan# 782
Delta R.T. -0.01 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Instrument :
BNA_F
ClientSampleId :
DUP

Tot Ion:152 Resp: 115887
Ion Ratio Lower Upper
152 100
150 158.9 126.2 189.2
115 65.1 52.2 78.2

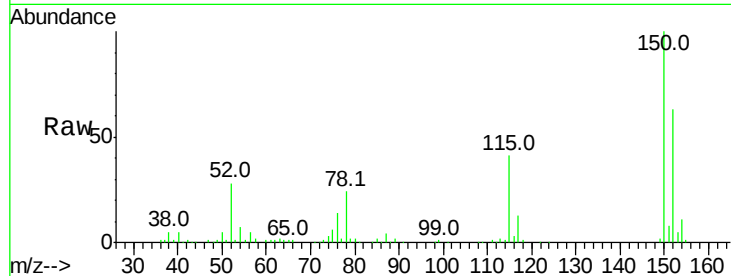


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

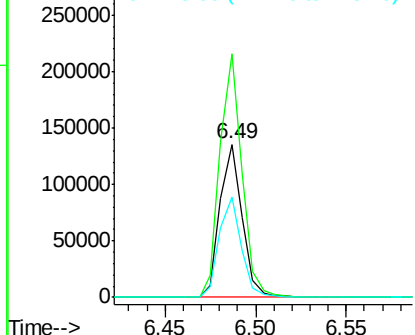



#5


2-Fluorophenol
Concen: 100.038 ng
RT: 5.09 min Scan# 545
Delta R.T. -0.01 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Tgt Ion:112 Resp: 769031
Ion Ratio Lower Upper
112 100
64 66.2 46.0 69.0
63 33.4 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

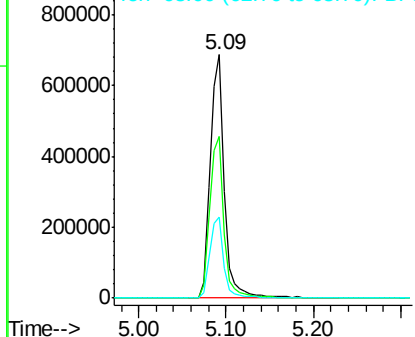

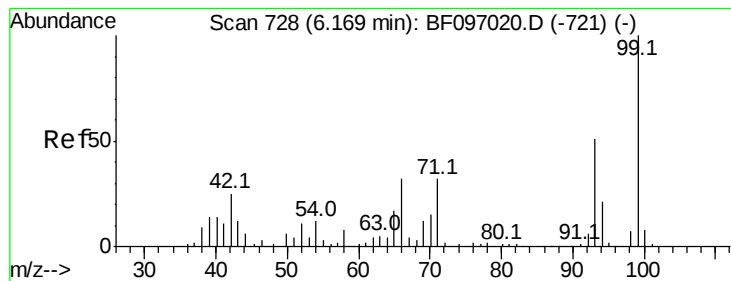

#7

Phenol-d6

Concen: 109.236 ng

RT: 6.15 min Scan# 725

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14

Instrument :

BNA_F

ClientSampleId :

DUP


Tot Ion: 99 Resp: 958668

Ion Ratio Lower Upper




99 100

42 23.8 13.5 20.3#

71 31.9 24.5 36.7

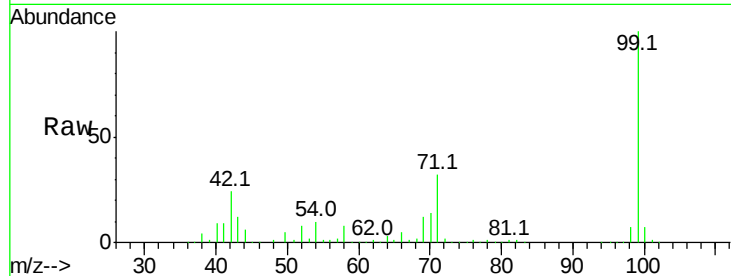

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

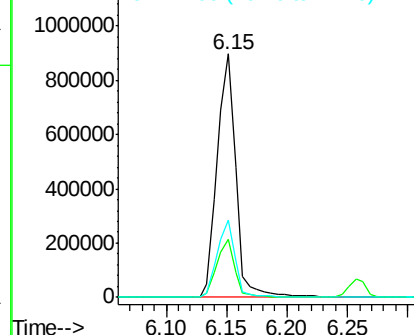

#10

Phenol

Concen: 2.560 ng

RT: 6.16 min Scan# 727

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14


Tgt Ion: 94 Resp: 26651

Ion Ratio Lower Upper



94 100

65 28.5 9.9 49.9

66 45.9 23.1 63.1



Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0

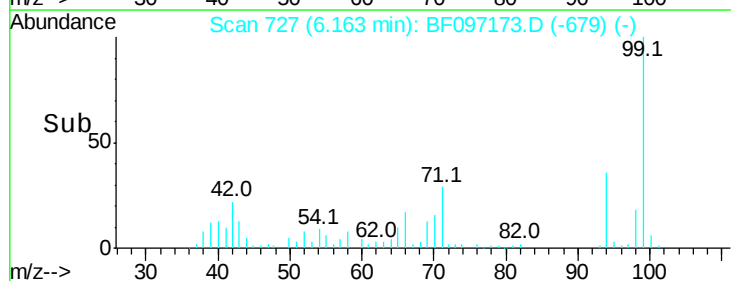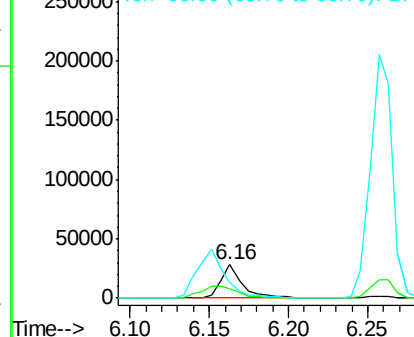



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.77 min Scan# 1000

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14

Instrument :

BNA_F

ClientSampleId :

DUP

Tot Ion:136 Resp: 439355


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 10.5 4.9 7.3#

68 6.1 4.1 6.1



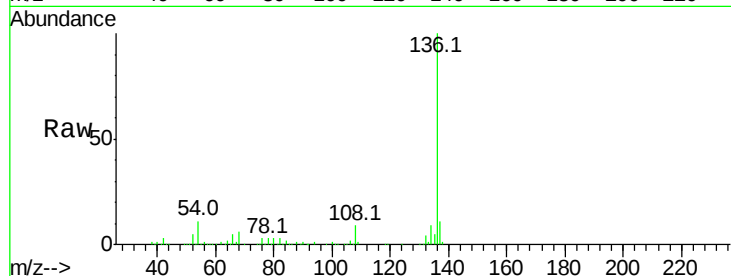


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

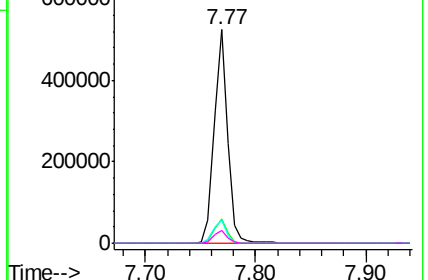

#23

Nitrobenzene-d5

Concen: 69.034 ng

RT: 7.06 min Scan# 879

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14


Tgt Ion: 82 Resp: 517022

Ion Ratio Lower Upper

82 100

128 49.2 34.0 51.0



54 65.4 42.2 63.2#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

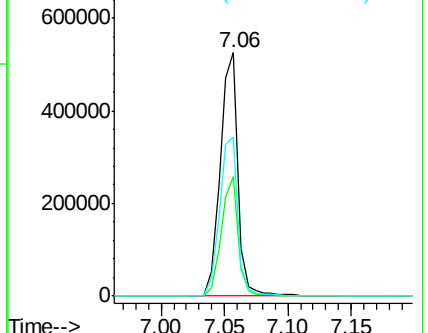







#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.51 min Scan# 1296
Delta R.T. -0.02 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Instrument :
BNA_F
ClientSampleId :
DUP

Tot Ion:164 Resp: 157800
Ion Ratio Lower Upper
164 100
162 105.1 82.6 123.8
160 45.0 36.2 54.2

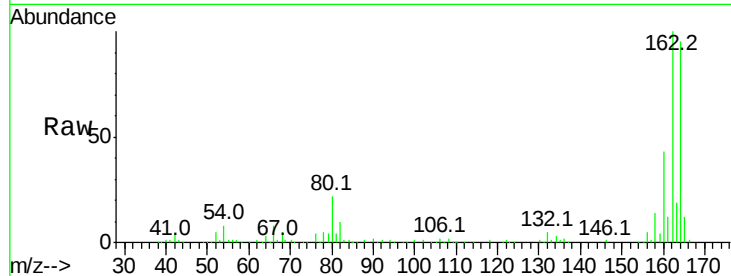


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

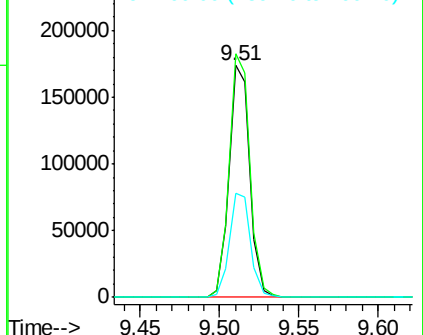
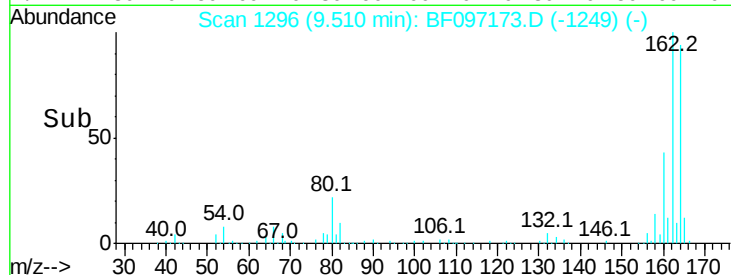


#41
2,4,6-Tribromophenol
Concen: 91.076 ng
RT: 10.30 min Scan# 1430
Delta R.T. -0.02 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Tgt Ion:330 Resp: 113551
Ion Ratio Lower Upper
330 100
332 94.5 76.6 115.0
141 40.2 31.4 47.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



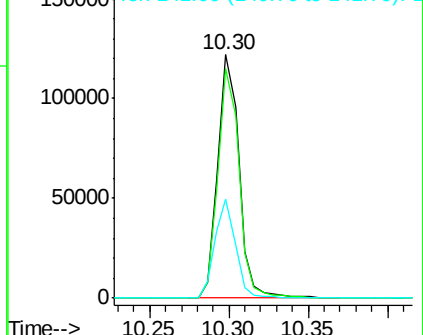





#44
 2-Fluorobiphenyl
 Concen: 75.044 ng
 RT: 8.85 min Scan# 1183
 Delta R.T. -0.02 min
 Lab File: BF097173.D
 Acq: 29 Jul 2017 00:14




Instrument :
 BNA_F
 ClientSampleId :
 DUP


Tot Ion:172 Resp: 697776
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.6 44.4
 170 24.6 19.8 29.8

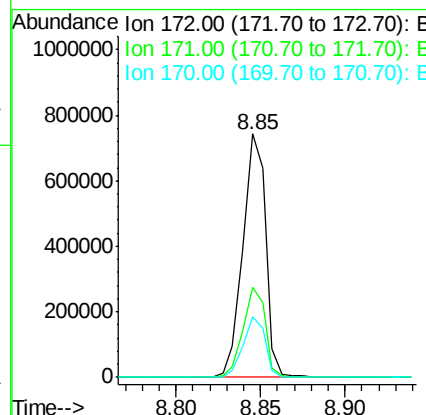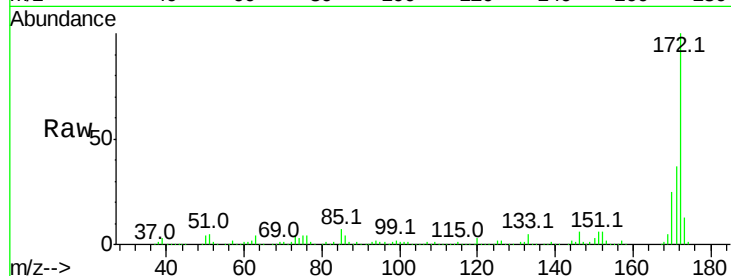

#49
 Dimethylphthalate
 Concen: 13.830 ng
 RT: 9.25 min Scan# 1251
 Delta R.T. -0.03 min
 Lab File: BF097173.D
 Acq: 29 Jul 2017 00:14

Tgt Ion:163 Resp: 165725
 Ion Ratio Lower Upper
 163 100
 194 2.9 2.6 4.0
 164 9.4 8.4 12.6

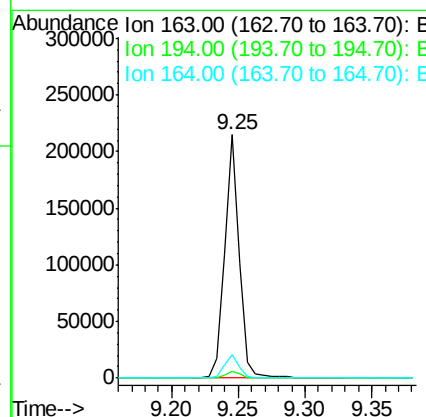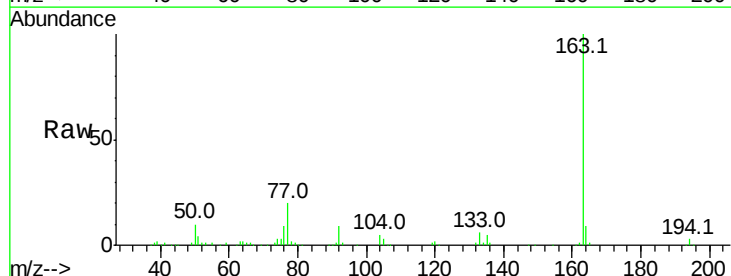


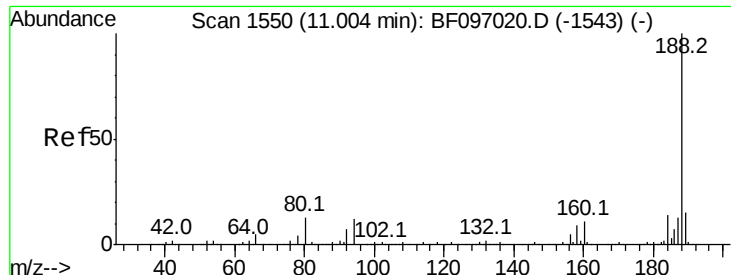




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 10.99 min Scan# 1547
Delta R.T. -0.02 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Instrument :
BNA_F
ClientSampleId :
DUP

Tot Ion:188 Resp: 211754
Ion Ratio Lower Upper
188 100
94 12.0 9.4 14.2
80 11.9 10.2 15.2

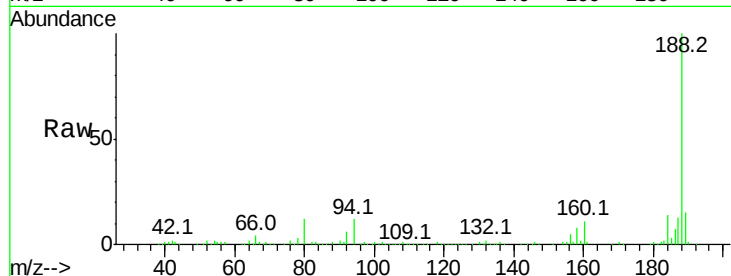


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


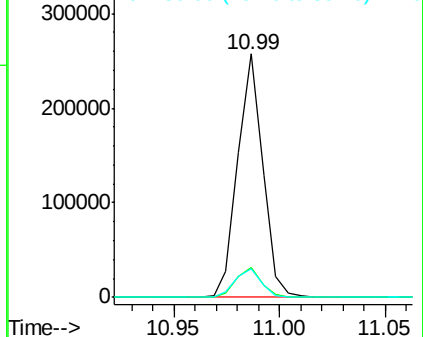



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.61 min Scan# 1993
Delta R.T. -0.02 min
Lab File: BF097173.D
Acq: 29 Jul 2017 00:14

Tgt Ion:240 Resp: 198252
Ion Ratio Lower Upper
240 100
120 15.4 5.8 8.8#
236 25.6 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

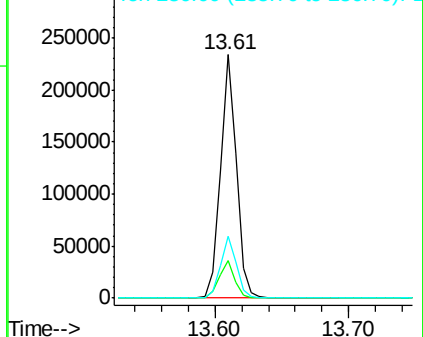



#78

Terphenyl-d14

Concen: 42.056 ng

RT: 12.57 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14

Instrument :

BNA_F

ClientSampleId :

DUP


Tot Ion:244 Resp: 408944

Ion Ratio Lower Upper

244 100

212 7.1 6.0 9.0




122 16.2 10.3 15.5#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

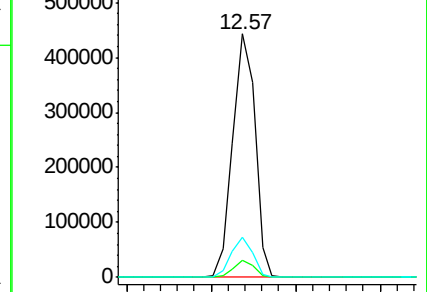

#86

Perylene-d12

Concen: 20.000 ng

RT: 14.96 min Scan# 2222

Delta R.T. -0.02 min

Lab File: BF097173.D

Acq: 29 Jul 2017 00:14


Tgt Ion:264 Resp: 162847

Ion Ratio Lower Upper

264 100

260 23.8 19.5 29.3

265 21.8 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

