


Data Path : Z:\HPCHEM1\BNA F\Data\BF072817\
 Data File : BF097141.D
 Acq On : 28 Jul 2017 8:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 31 15:18:22 2017

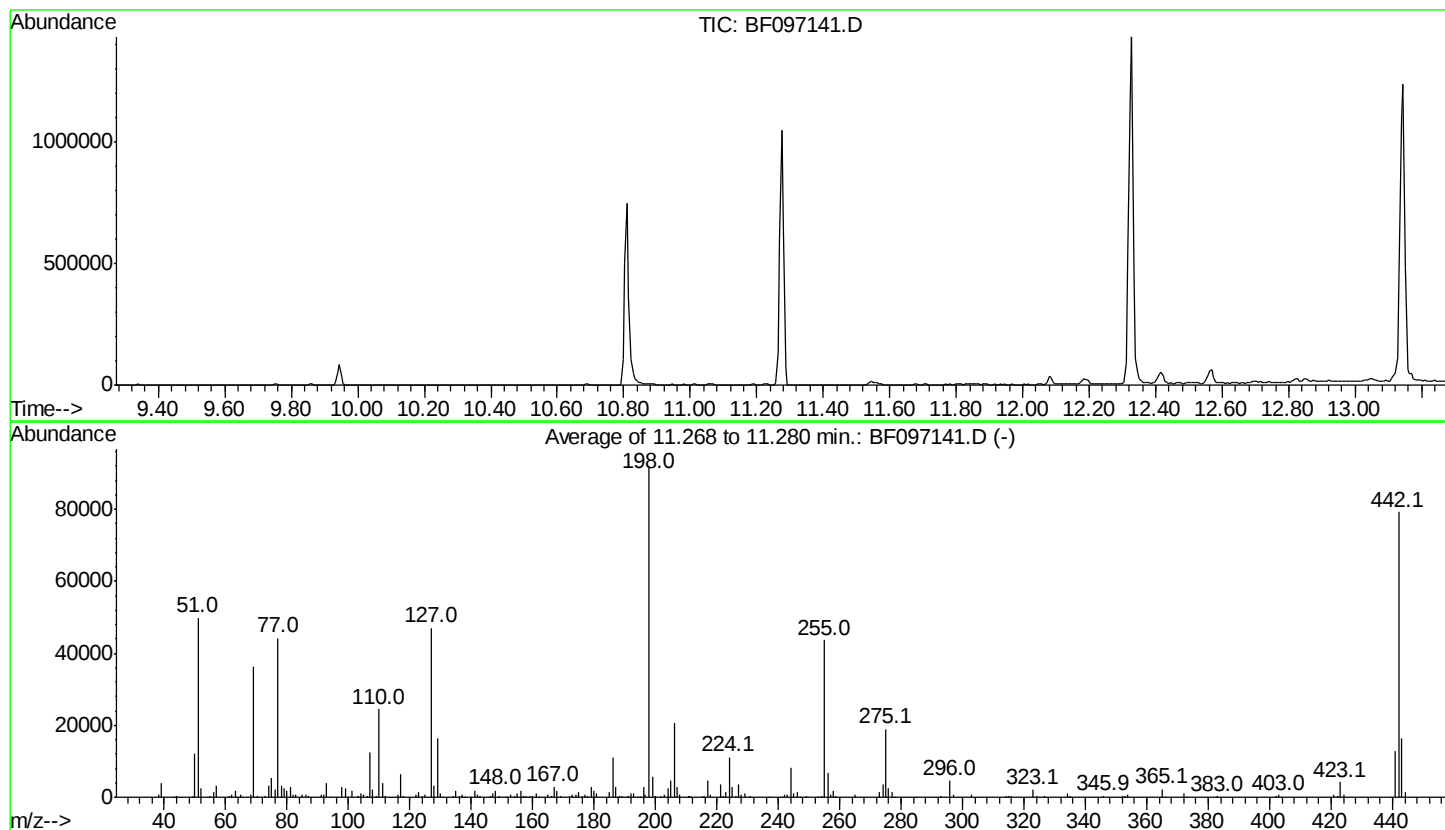

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	49893	PASS
68	69	0.00	2	1.8	653	PASS
69	198	0.00	100	39.4	36336	PASS
70	69	0.00	2	0.6	229	PASS
127	198	10	80	51.1	47077	PASS
197	198	0.00	2	0.7	650	PASS
198	198	100	100	100.0	92168	PASS
199	198	5	9	6.4	5861	PASS
275	198	10	60	20.6	19013	PASS
365	198	1	100	2.5	2319	PASS
441	442	0.01	24	16.1	12798	PASS
442	198	50	100	86.0	79250	PASS
443	442	15	24	20.6	16364	PASS