

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072820\
 Data File : BF121068.D
 Acq On : 28 Jul 2020 14:21
 Operator : JU/CG
 Sample : L3434-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 11936

Quant Time: Jul 28 14:51:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	153446	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	555412	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	313893	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	644802	20.00	ng	0.00
76) Chrysene-d12	13.97	240	559717	20.00	ng	0.00
86) Perylene-d12	15.42	264	500326	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	780477	83.38	ng	0.00
7) Phenol-d6	6.45	99	938343	77.61	ng	0.00
23) Nitrobenzene-d5	7.37	82	584307	60.87	ng	0.00
42) 2,4,6-Tribromophenol	10.63	330	316249	92.04	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	1182563	56.25	ng	0.00
79) Terphenyl-d14	12.92	244	1323341	51.39	ng	0.00
Target Compounds						
9) Benzaldehyde	6.44	77	1323	Below Cal		Qvalue # 1
19) n-Nitroso-di-n-propylamine	7.37	70	77266	11.238	ng	# 77
25) Isophorone	7.37	82	584298	30.501	ng	# 63
50) Dimethylphthalate	9.56	163	154456	6.821	ng	99
57) 2,4-Dinitrotoluene	9.85	165	40189	6.290	ng	# 27
65) 4,6-Dinitro-2-methylphenol	10.63	198	572	3.984	ng	# 1
67) 4-Bromophenyl-phenylether	10.63	248	18277	2.542	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072820\
Data File : BF121068.D
Acq On : 28 Jul 2020 14:21
Operator : JU/CG
Sample : L3434-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
11936

Quant Time: Jul 28 14:51:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

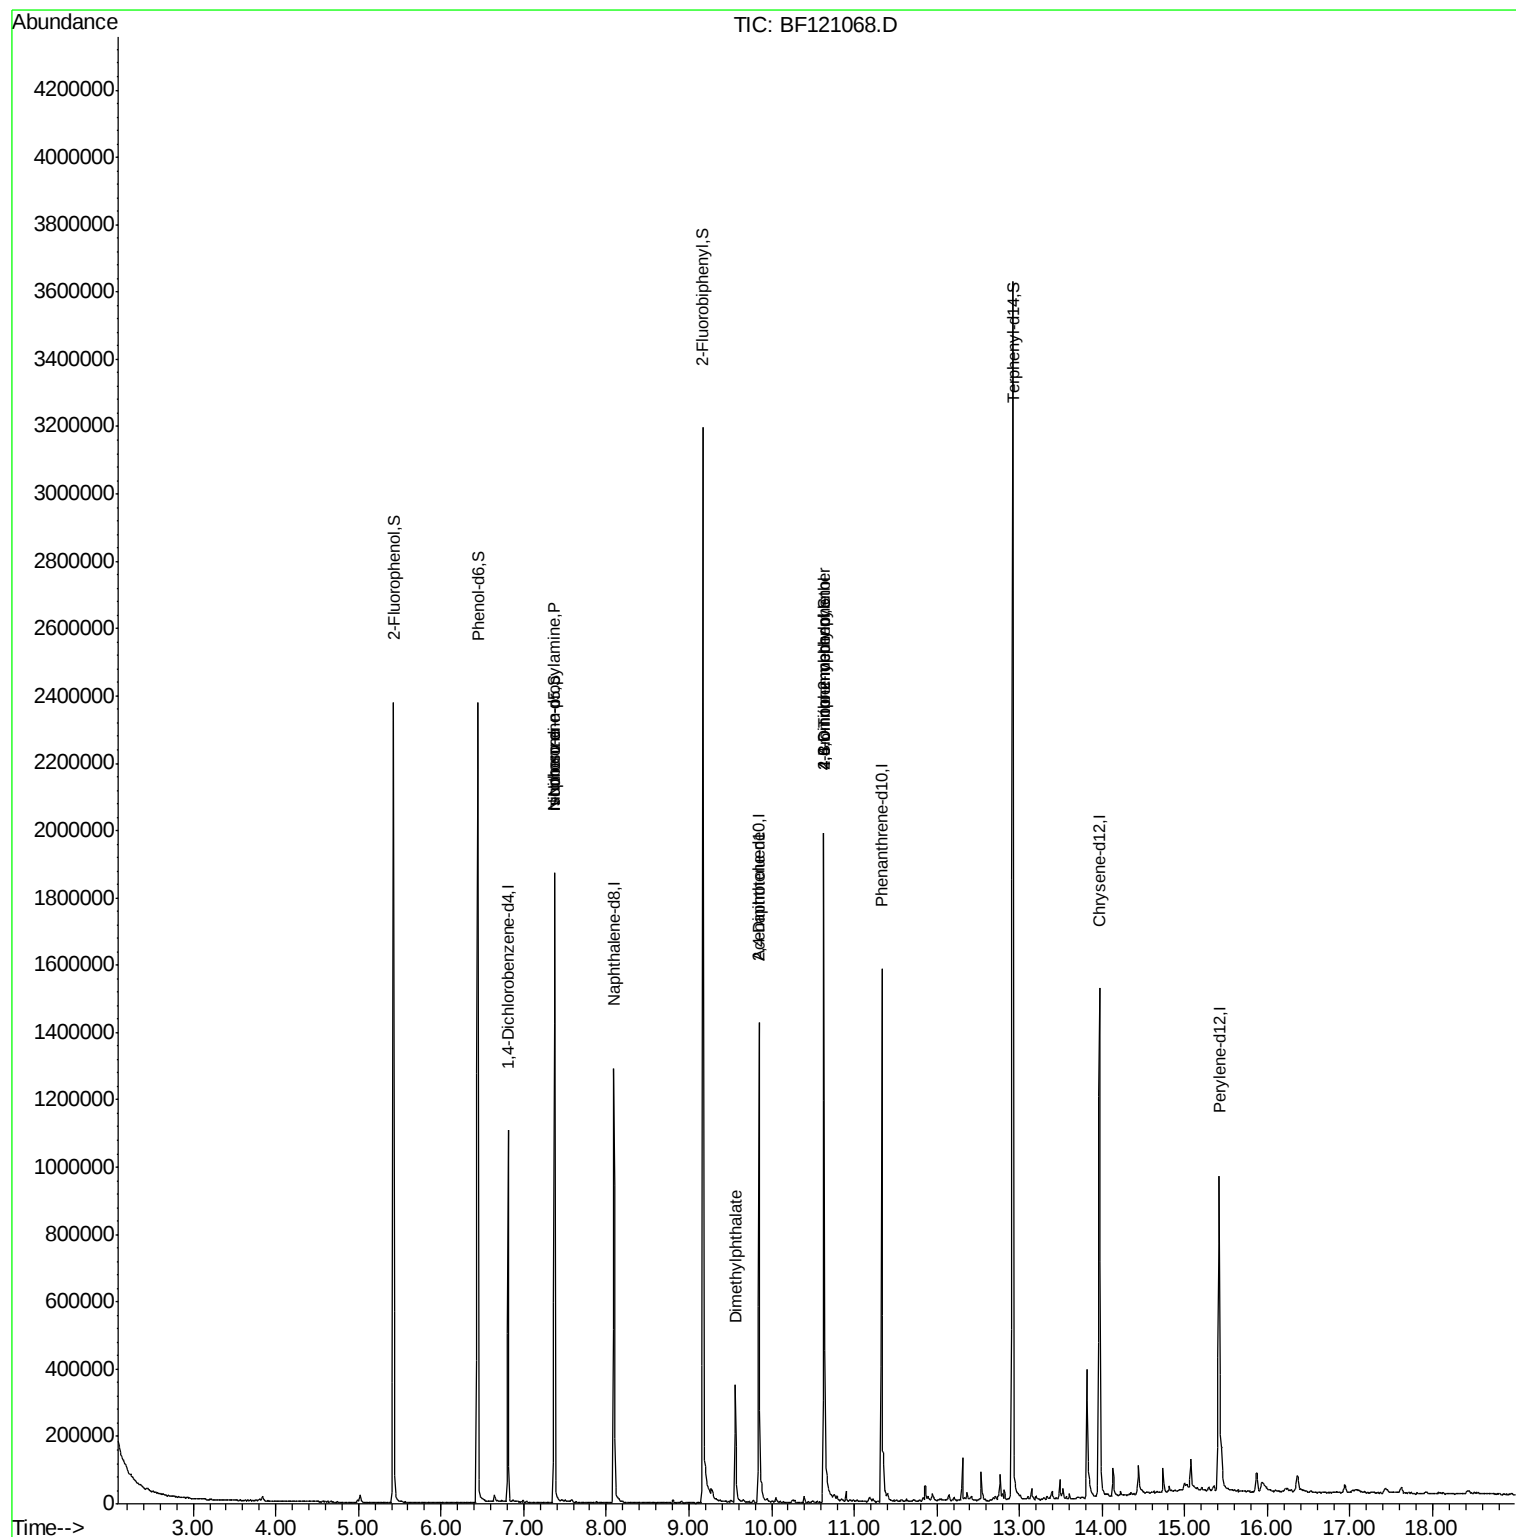

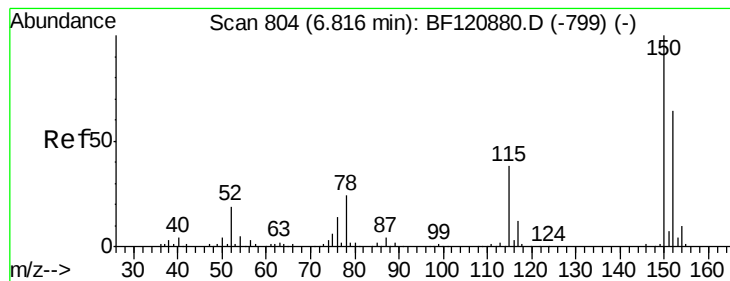


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.81 min Scan# 803
Delta R.T. -0.01 min
Lab File: BF121068.D
Acq: 28 Jul 2020 14:21

Instrument :
BNA_F
ClientSampleId :
11936

Tot Ion:152 Resp: 153446
Ion Ratio Lower Upper
152 100
150 156.7 125.0 187.6
115 59.9 47.0 70.4

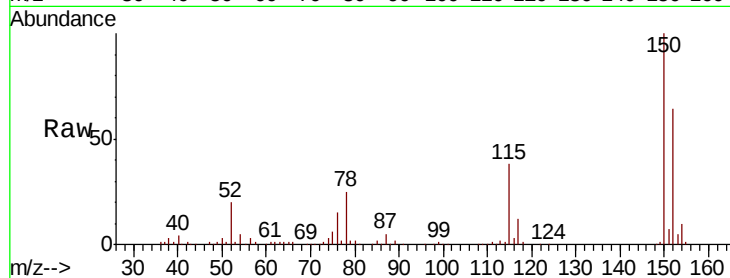


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

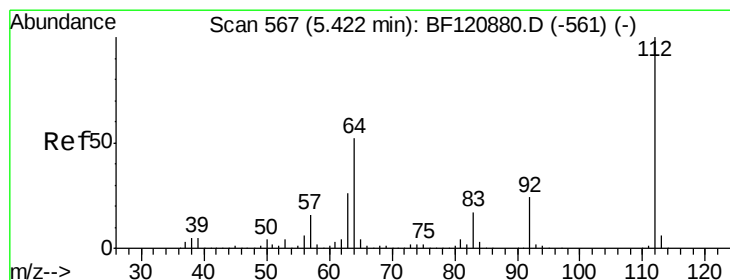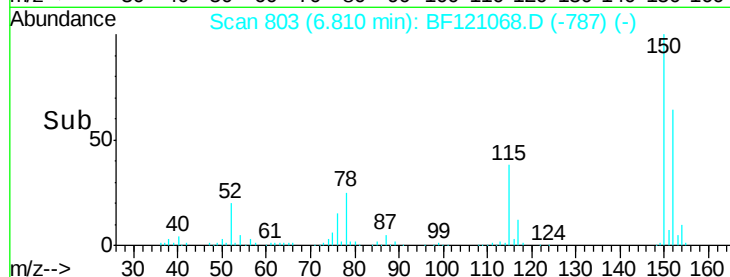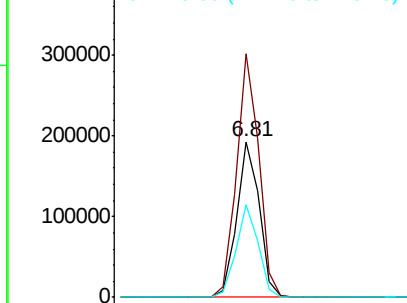



#5




2-Fluorophenol
Concen: 83.383 ng
RT: 5.43 min Scan# 568
Delta R.T. 0.01 min
Lab File: BF121068.D
Acq: 28 Jul 2020 14:21

Tgt Ion:112 Resp: 780477
Ion Ratio Lower Upper
112 100
64 51.1 41.3 61.9
63 26.2 21.1 31.7

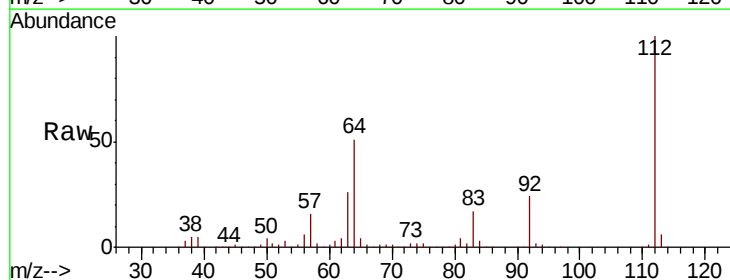

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

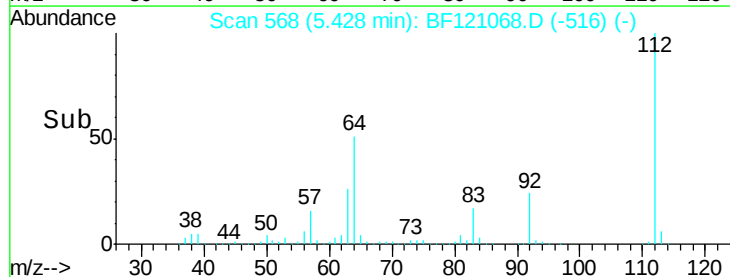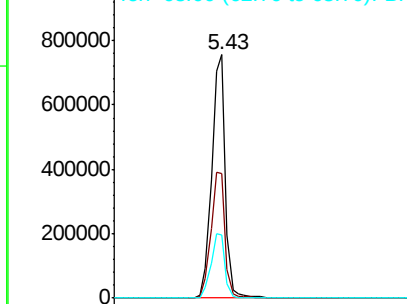

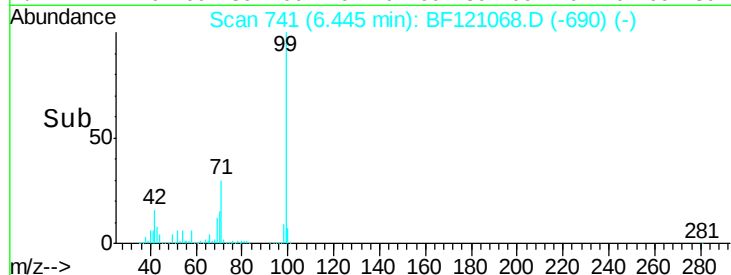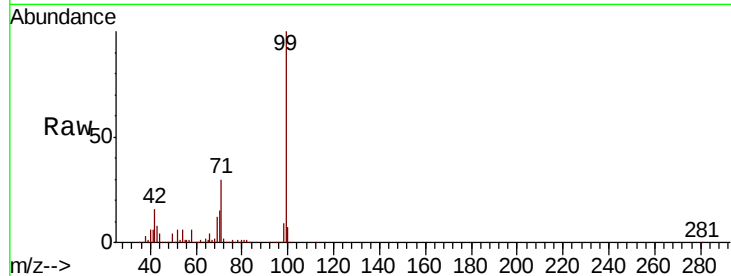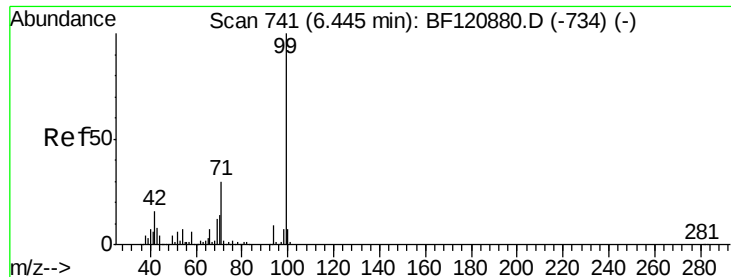

#7

Phenol-d6

Concen: 77.607 ng

RT: 6.45 min Scan# 741

Delta R.T. 0.00 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampleId :

11936




Tot Ion: 99 Resp: 938343

Ion Ratio Lower Upper

99 100

42 16.1 13.1 19.7

71 30.5 24.2 36.4

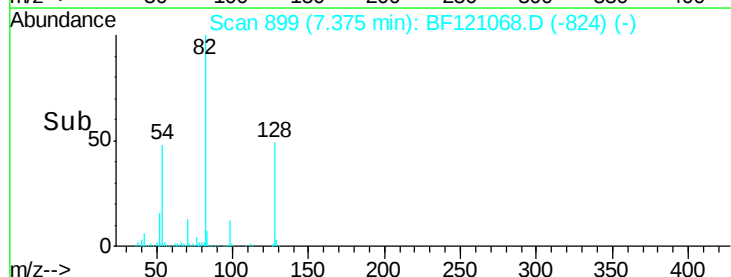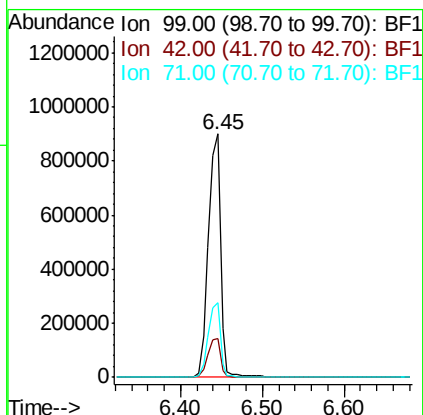

#19

n-Nitroso-di-n-propylamine

Concen: 11.238 ng

RT: 7.37 min Scan# 899

Delta R.T. 0.14 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Tgt Ion: 70 Resp: 77266


Ion Ratio Lower Upper

70 100

42 44.7 44.0 66.0

101 0.0 7.8 11.6#

130 2.2 18.7 28.1#

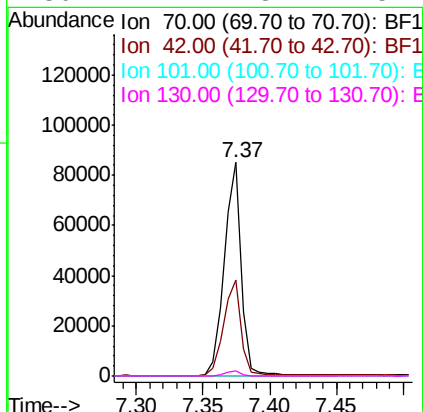



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampled :

11936

Tot Ion:136 Resp: 555412


Ion Ratio Lower Upper

136 100

137 11.2 9.3 13.9

54 7.6 6.3 9.5

68 6.3 5.0 7.4





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

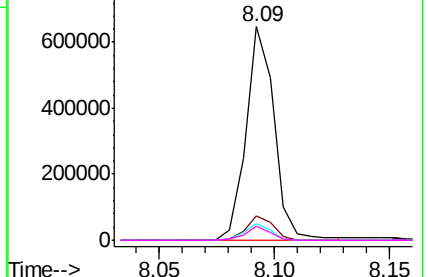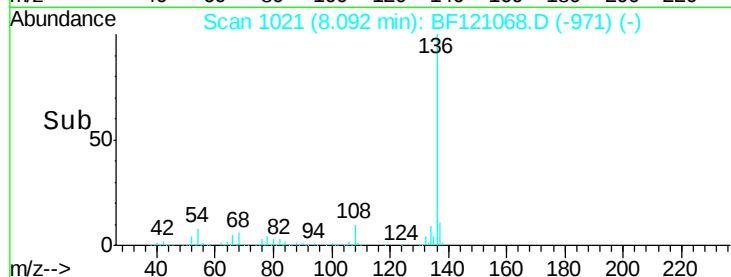

#23

Nitrobenzene-d5

Concen: 60.873 ng

RT: 7.37 min Scan# 899

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21


Tgt Ion: 82 Resp: 584307

Ion Ratio Lower Upper

82 100

128 49.2 38.2 57.4



54 48.1 38.7 58.1



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

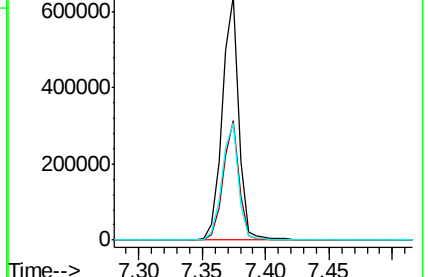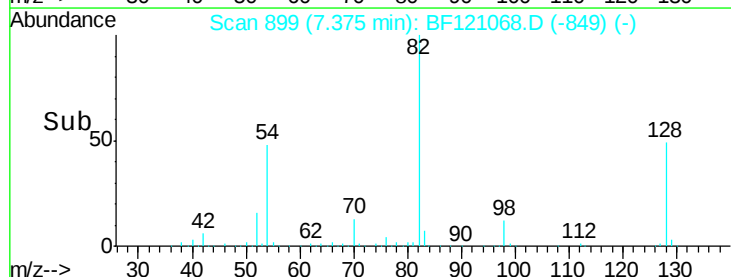



#25

Isophorone

Concen: 30.501 ng

RT: 7.37 min Scan# 899

Delta R.T. -0.26 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampleId :

11936





Tot Ion: 82 Resp: 584298

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#

138 0.0 15.6 23.4#

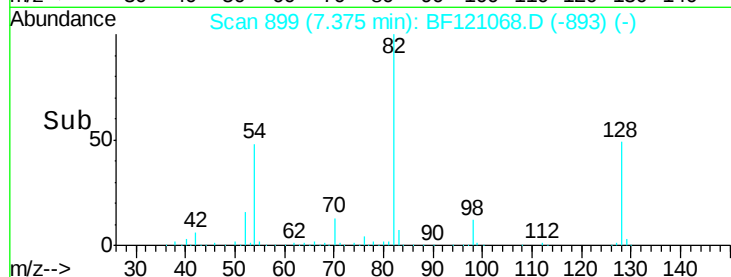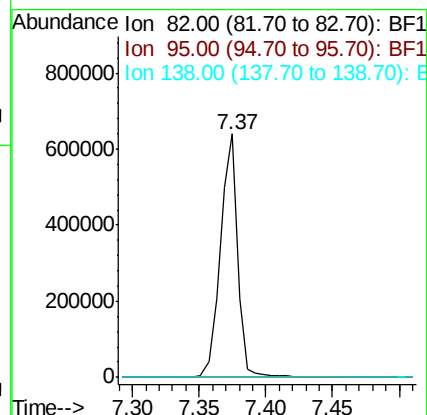

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1319

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21




Tgt Ion: 164 Resp: 313893


Ion Ratio Lower Upper

164 100

162 100.6 81.2 121.8

160 45.6 36.9 55.3

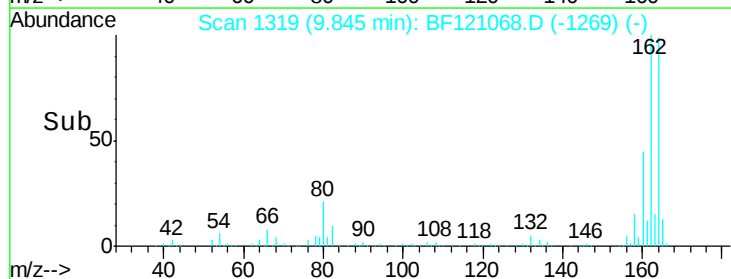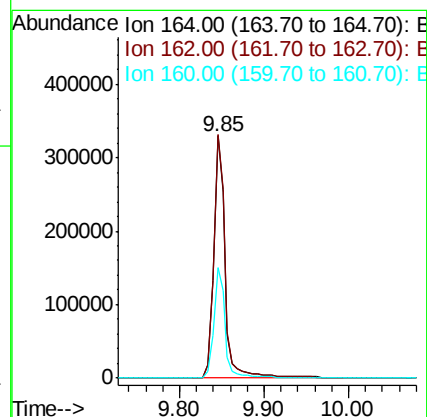

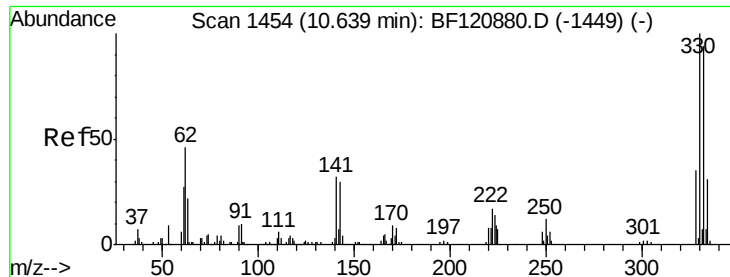

#42

2,4,6-Tribromophenol

Concen: 92.043 ng

RT: 10.63 min Scan# 1453

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampleId :

11936


Tot Ion:330 Resp: 316249

Ion Ratio Lower Upper

330 100

332 96.0 75.5 113.3




141 29.8 25.7 38.5

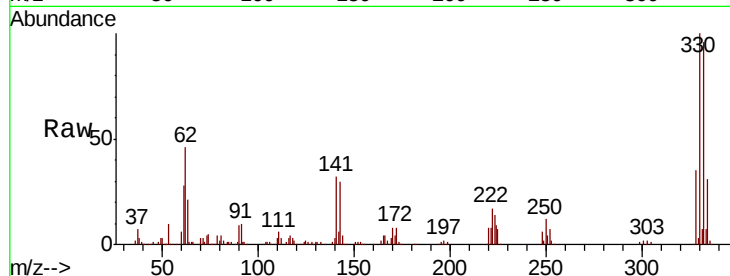

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

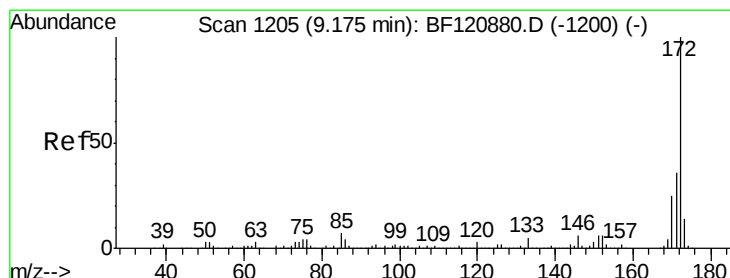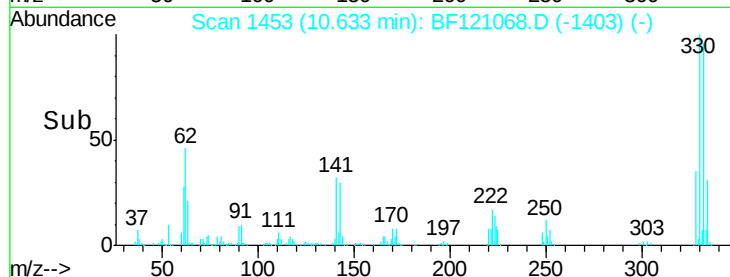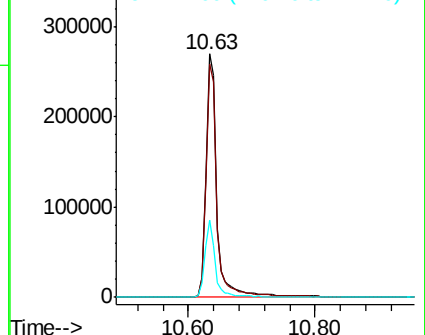

#45

2-Fluorobiphenyl

Concen: 56.249 ng

RT: 9.17 min Scan# 1204

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21


Tgt Ion:172 Resp: 1182563

Ion Ratio Lower Upper

172 100

171 35.7 29.0 43.4



170 24.0 19.6 29.4

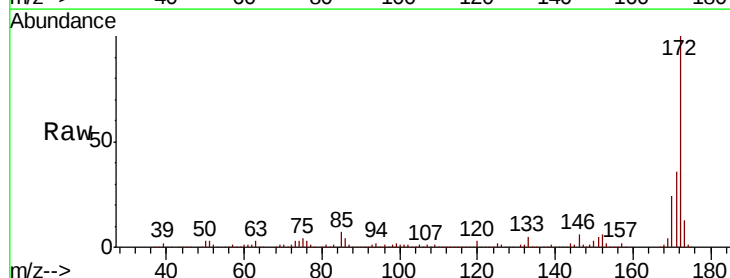


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

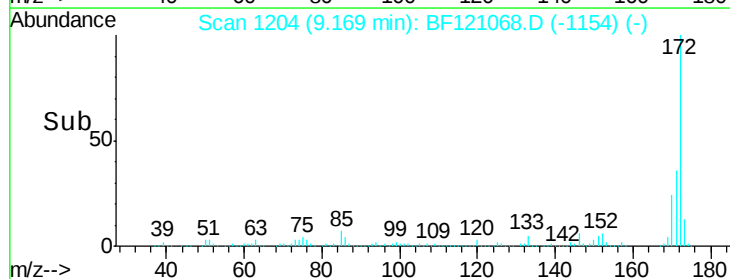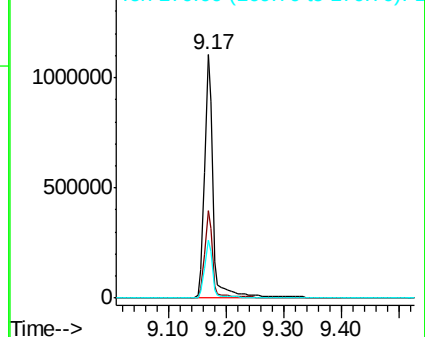

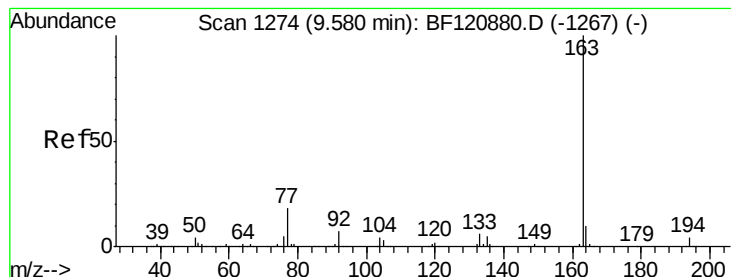

#50

Dimethylphthalate

Concen: 6.821 ng

RT: 9.56 min Scan# 1271

Delta R.T. -0.02 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampled :

11936


Tot Ion:163 Resp: 154456

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.3 7.9 11.9






Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

Time-->

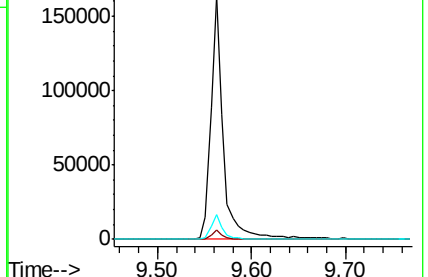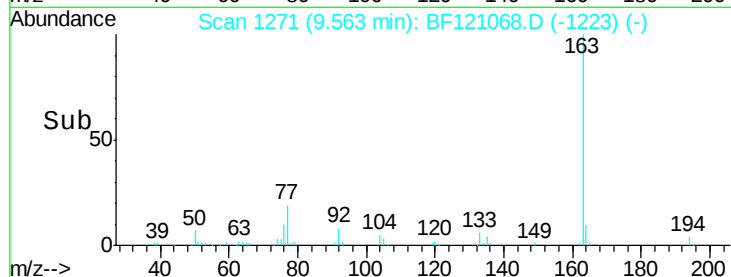

#57

2,4-Dinitrotoluene

Concen: 6.290 ng

RT: 9.85 min Scan# 1319

Delta R.T. -0.19 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Tgt Ion:165 Resp: 40189


Ion Ratio Lower Upper

165 100

63 1.1 29.4 44.2#

89 1.2 53.4 80.0#

182 0.0 1.8 2.6#





Abundance Ion 165.00 (164.70 to 165.70): E


Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

Time-->

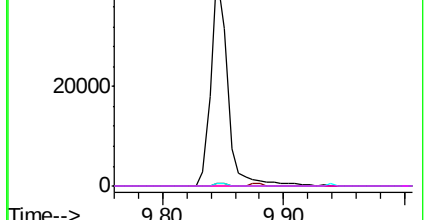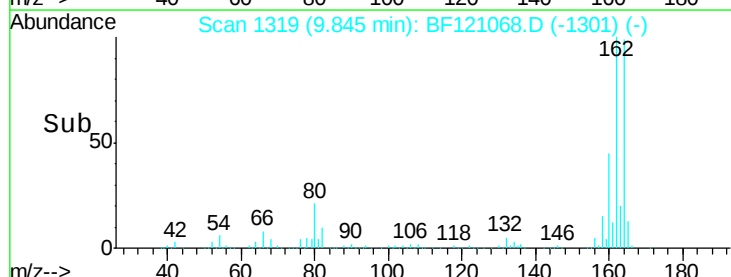

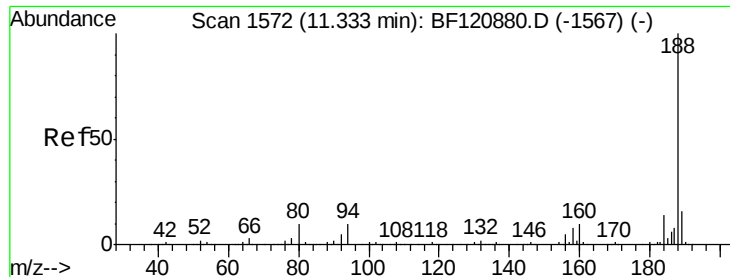

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1572

Delta R.T. 0.00 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampleId :

11936


Tot Ion:188 Resp: 644802

Ion Ratio Lower Upper

188 100

94 8.6 8.0 12.0




80 8.5 8.3 12.5

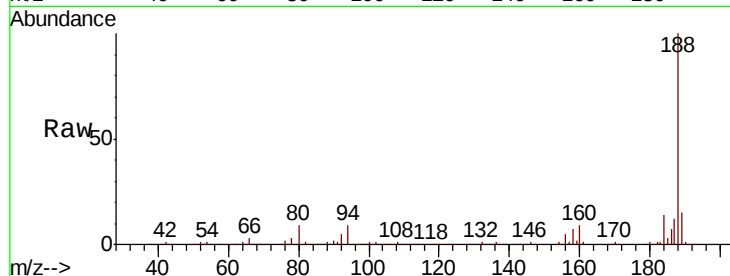

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

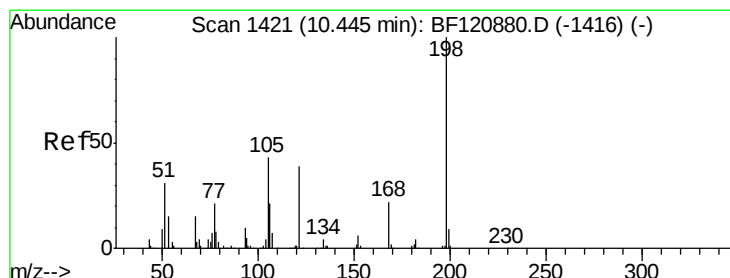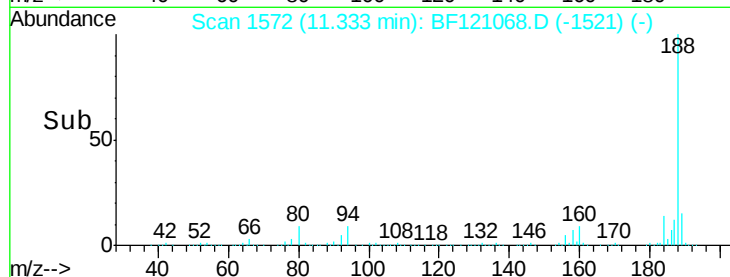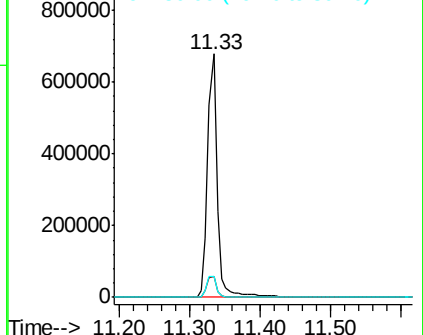

#65

4,6-Dinitro-2-methylphenol

Concen: 3.984 ng

RT: 10.63 min Scan# 1453

Delta R.T. 0.19 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21


Tgt Ion:198 Resp: 572

Ion Ratio Lower Upper

198 100

51 180.8 19.5 59.5#



105 193.1 24.4 64.4#

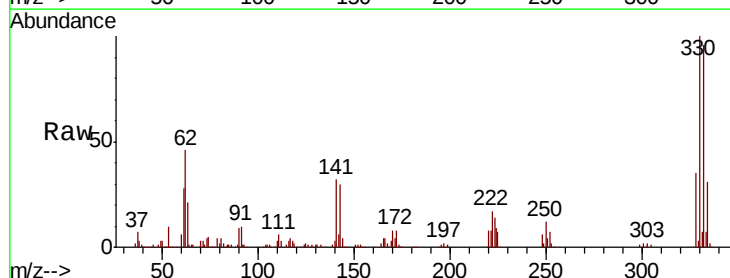


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

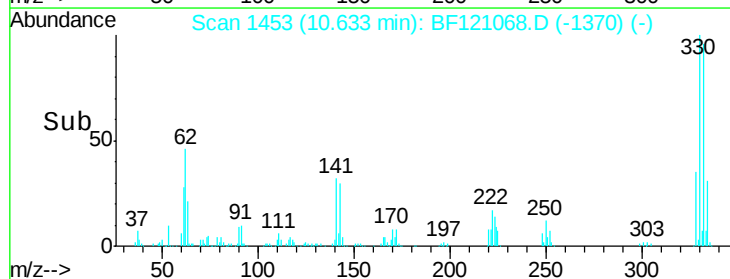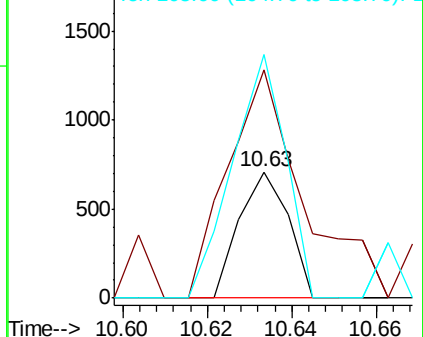


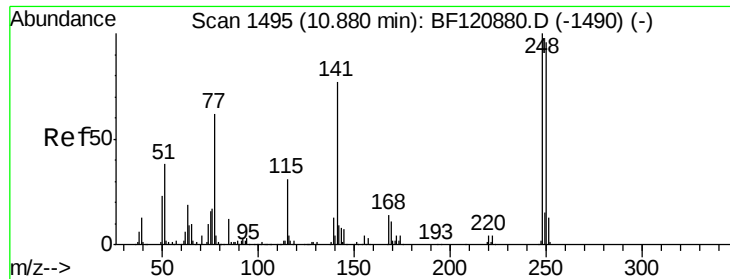




#67
 4-Bromophenyl-phenylether
 Concen: 2.542 ng
 RT: 10.63 min Scan# 1453
 Delta R.T. -0.25 min
 Lab File: BF121068.D
 Acq: 28 Jul 2020 14:21

Instrument :
 BNA_F
 ClientSampled :
 11936

Tot Ion:248 Resp: 18277
 Ion Ratio Lower Upper
 248 100
 250 196.2 77.1 115.7#
 141 497.8 61.2 91.8#

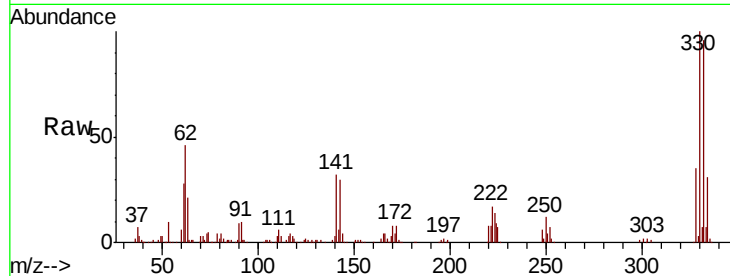


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

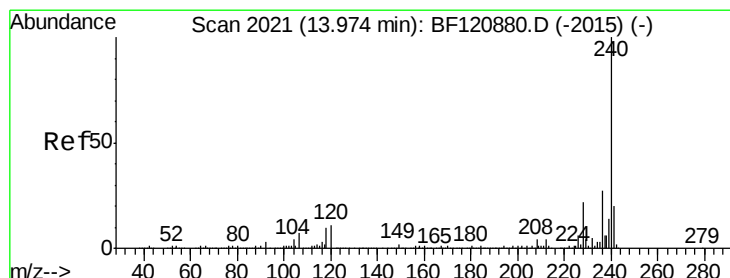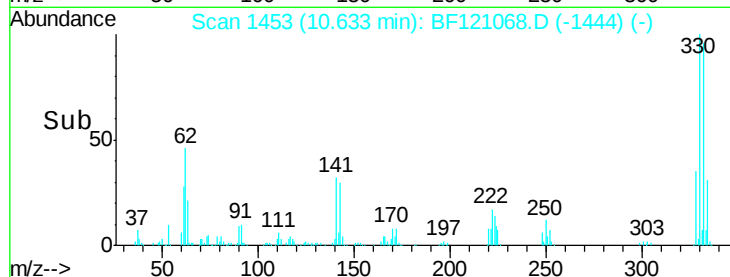
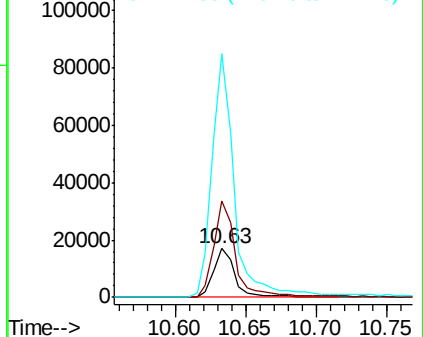


#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.97 min Scan# 2020
 Delta R.T. -0.01 min
 Lab File: BF121068.D
 Acq: 28 Jul 2020 14:21

Tgt Ion:240 Resp: 559717
 Ion Ratio Lower Upper
 240 100
 120 10.8 9.0 13.4
 236 27.0 21.7 32.5

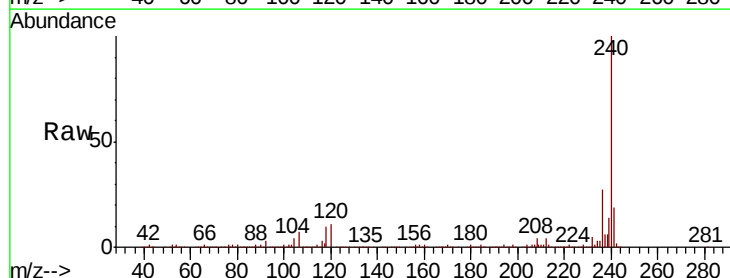

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

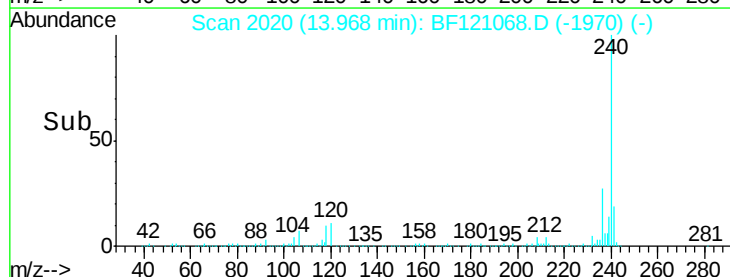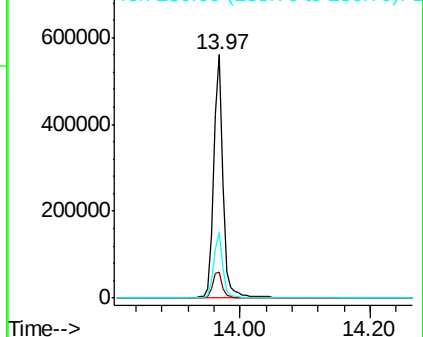



#79

Terphenyl-d14

Concen: 51.395 ng

RT: 12.92 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21

Instrument :

BNA_F

ClientSampleId :

11936


Tot Ion:244 Resp: 1323341

Ion Ratio Lower Upper

244 100

212 6.9 5.6 8.4




122 10.6 8.9 13.3



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

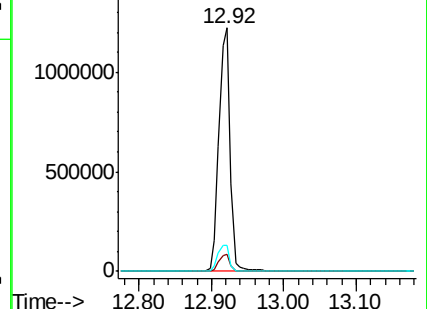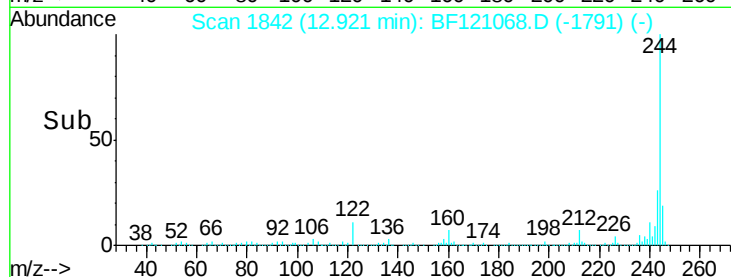

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.42 min Scan# 2266

Delta R.T. -0.01 min

Lab File: BF121068.D

Acq: 28 Jul 2020 14:21


Tgt Ion:264 Resp: 500326

Ion Ratio Lower Upper

264 100

260 24.3 20.0 30.0

265 21.0 17.4 26.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

