

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072820\
 Data File : BF121092.D
 Acq On : 29 Jul 2020 3:00
 Operator : JU/CG
 Sample : L3414-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 61820

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	564	567	581	rBV	496271	497644	29.72%	4.203%
2	6.445	738	741	753	rBV	493671	477242	28.50%	4.031%
3	6.810	800	803	807	rBV	1112758	975188	58.23%	8.236%
4	7.369	895	898	909	rBV	334248	323804	19.34%	2.735%
5	8.098	1018	1022	1025	rBV	1434294	1185085	70.77%	10.009%
6	8.145	1028	1030	1044	rVB5	14596	37209	2.22%	0.314%
7	9.169	1201	1204	1216	rBV	670387	615531	36.76%	5.199%
8	9.569	1268	1272	1277	rBV	39361	46167	2.76%	0.390%
9	9.710	1293	1296	1300	rBV	42135	35262	2.11%	0.298%
10	9.851	1316	1320	1335	rBV	1400788	1385257	82.72%	11.700%
11	10.639	1450	1454	1466	rBV	368794	421557	25.17%	3.560%
12	10.763	1471	1475	1482	rVB3	19919	29282	1.75%	0.247%
13	11.233	1552	1555	1560	rVB	31212	35698	2.13%	0.301%
14	11.333	1568	1572	1582	rBV	1577077	1674659	100.00%	14.144%
15	11.410	1582	1585	1588	rVB	43534	45392	2.71%	0.383%
16	11.575	1610	1613	1617	rBV3	18629	31055	1.85%	0.262%
17	11.833	1655	1657	1659	rBV	26837	24730	1.48%	0.209%
18	11.863	1659	1662	1668	rVB	40287	42116	2.51%	0.356%
19	11.945	1673	1676	1679	rBV	63763	69832	4.17%	0.590%
20	12.263	1727	1730	1732	rBV3	27939	33541	2.00%	0.283%
21	12.316	1736	1739	1740	rBV2	31746	32925	1.97%	0.278%
22	12.386	1748	1751	1753	rBV	43261	46382	2.77%	0.392%
23	12.545	1775	1778	1782	rBV	279822	243907	14.56%	2.060%
24	12.774	1814	1817	1823	rVB	355677	339473	20.27%	2.867%
25	12.916	1838	1841	1848	rBV	931324	832814	49.73%	7.034%
26	13.974	2017	2021	2023	rBV	1136381	1176507	70.25%	9.936%
27	15.427	2264	2268	2278	rVB	819674	1182026	70.58%	9.983%


Sum of corrected areas: 11840285

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072820\
Data File : BF121092.D
Acq On : 29 Jul 2020 3:00
Operator : JU/CG
Sample : L3414-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
61820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

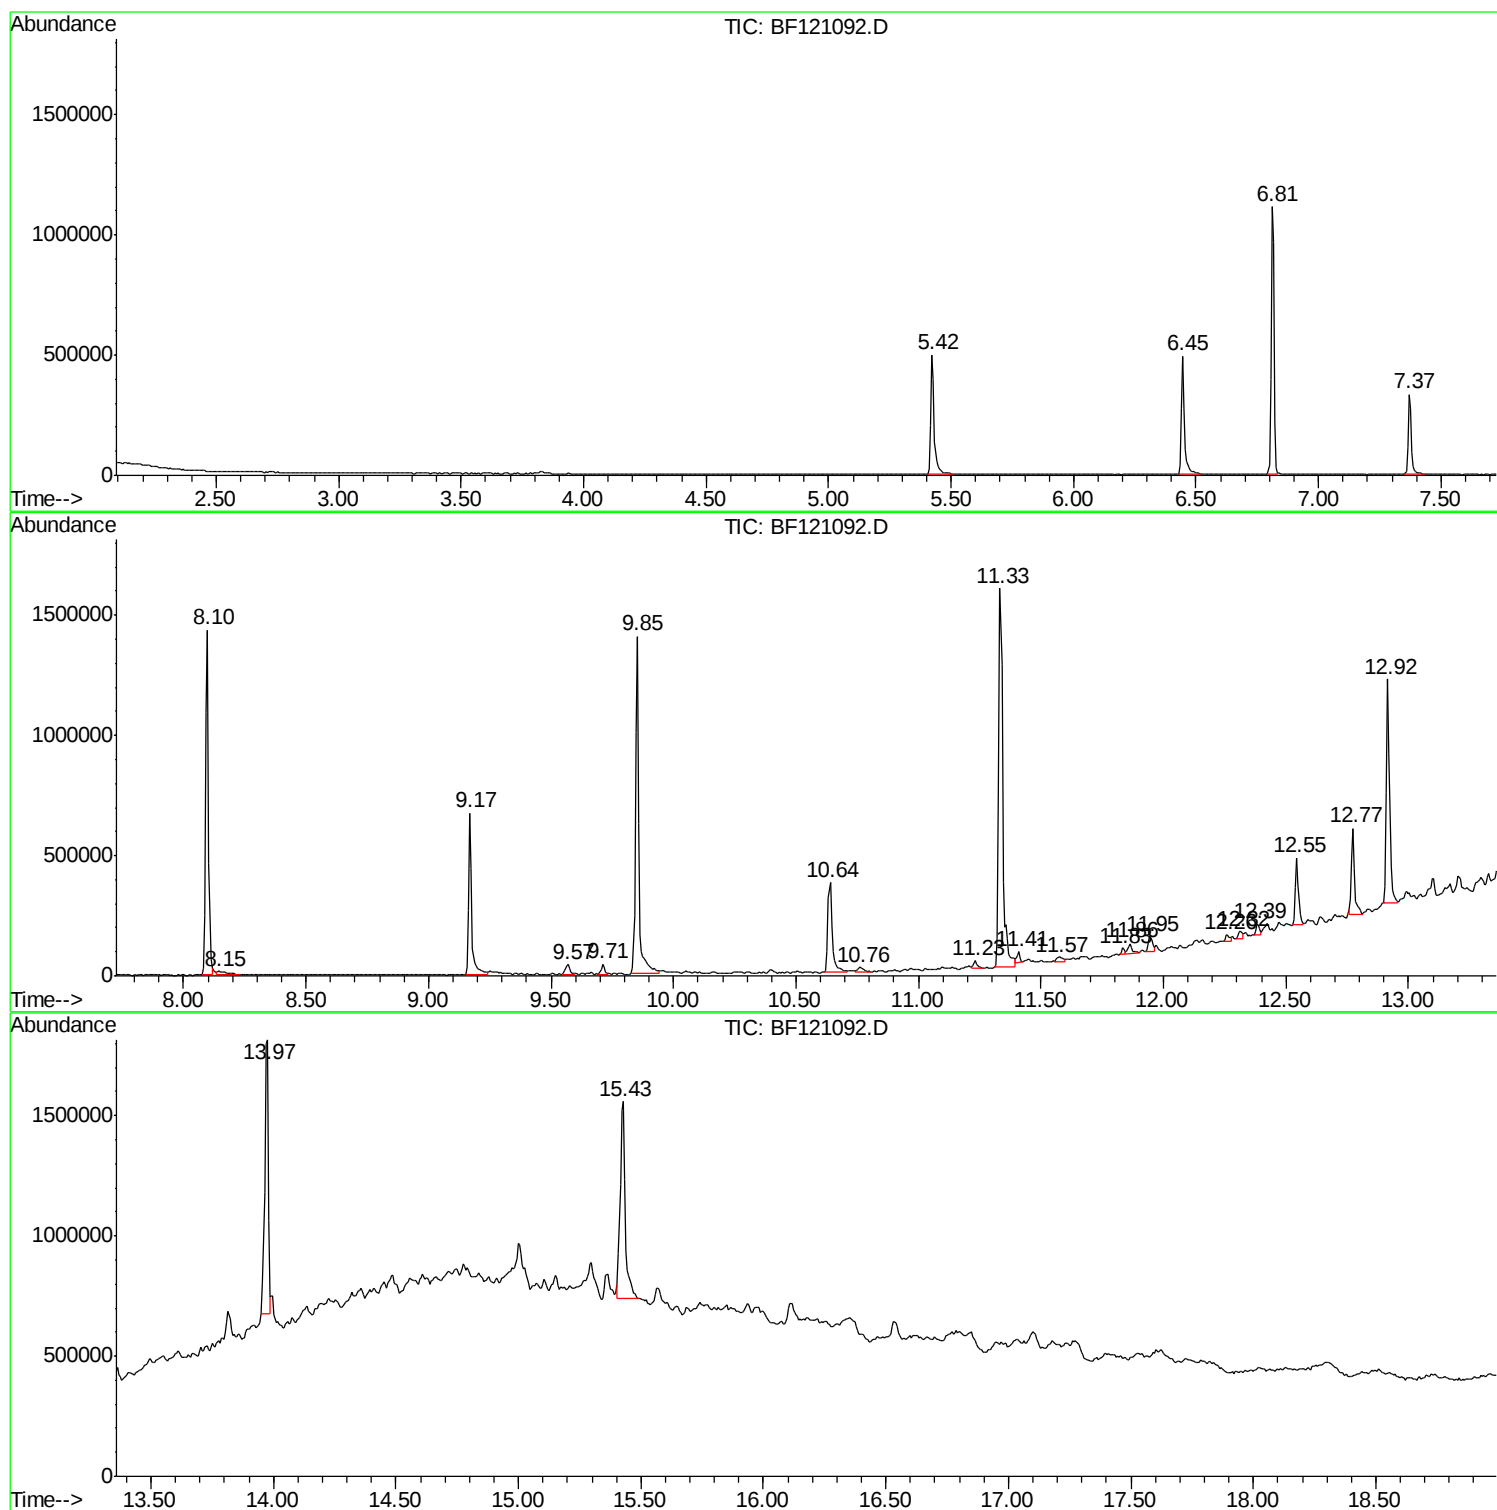

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072820\
Data File : BF121092.D
Acq On : 29 Jul 2020 3:00
Operator : JU/CG
Sample : L3414-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
61820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072820\
Data File : BF121092.D
Acq On : 29 Jul 2020 3:00
Operator : JU/CG
Sample : L3414-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
61820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc