


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072820\
 Data File : BF121058.D
 Acq On : 28 Jul 2020 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 14:20:32 2020

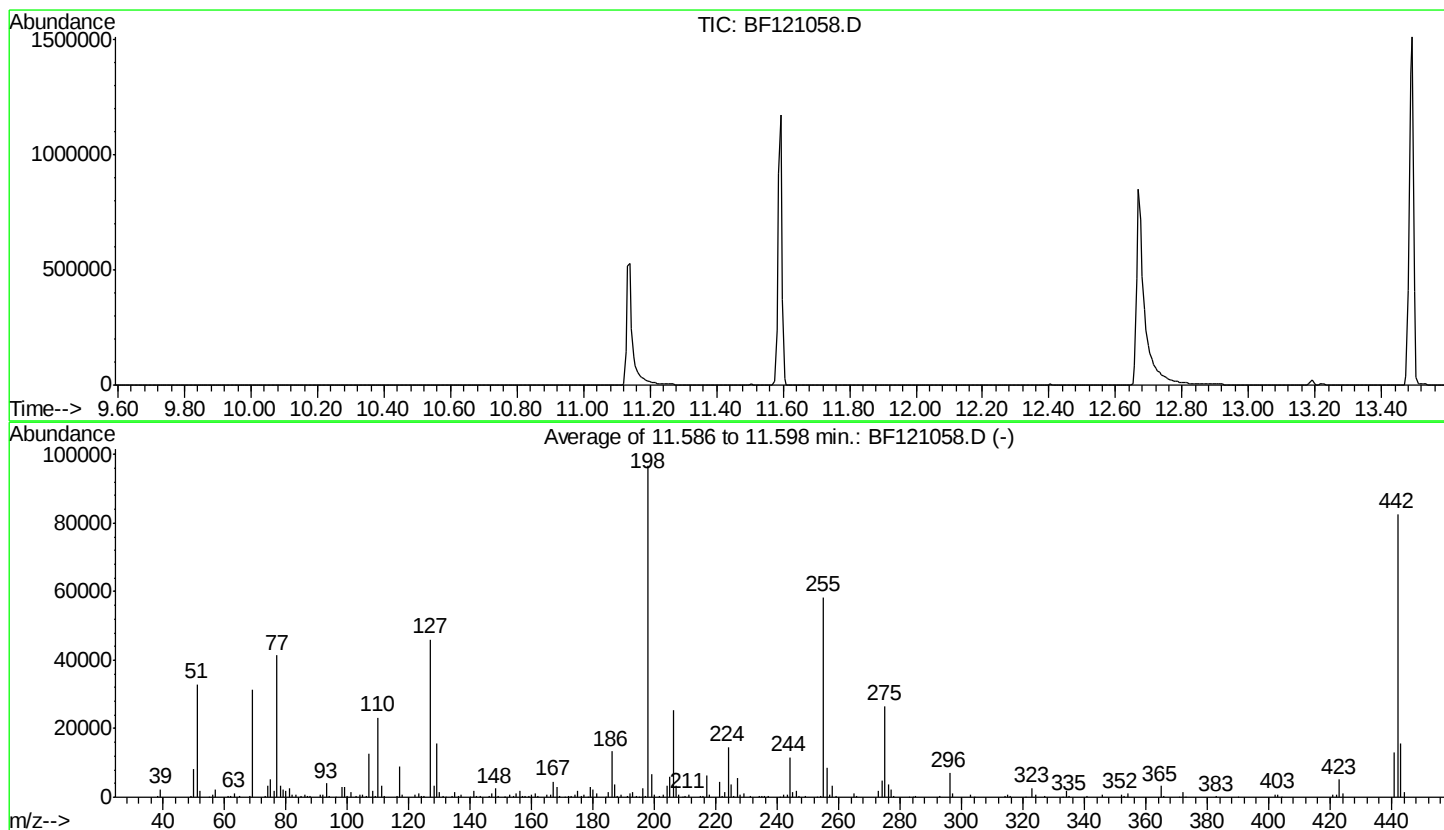

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	32954	PASS
68	69	0.00	2	1.5	480	PASS
69	198	0.00	100	32.4	31348	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	45945	PASS
197	198	0.00	2	0.6	564	PASS
198	198	100	100	100.0	96744	PASS
199	198	5	9	7.0	6741	PASS
275	198	10	60	27.5	26557	PASS
365	198	1	100	3.5	3340	PASS
441	198	0.01	100	13.4	13011	PASS
442	198	50	100	85.4	82634	PASS
443	442	15	24	19.1	15785	PASS