
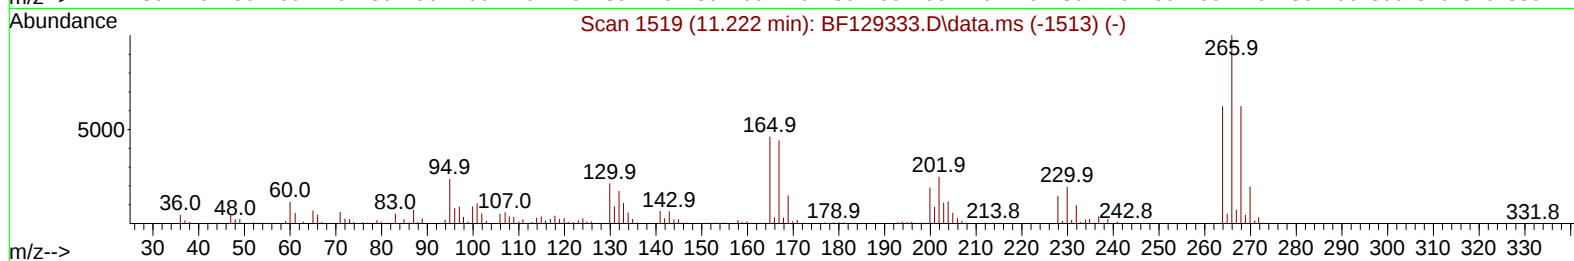
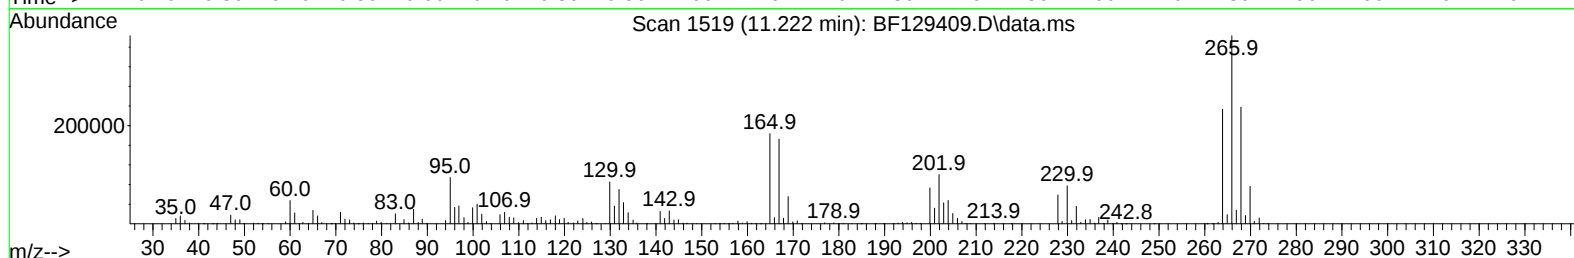


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129409.D
 Acq On : 28 Jul 2022 15:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:38:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

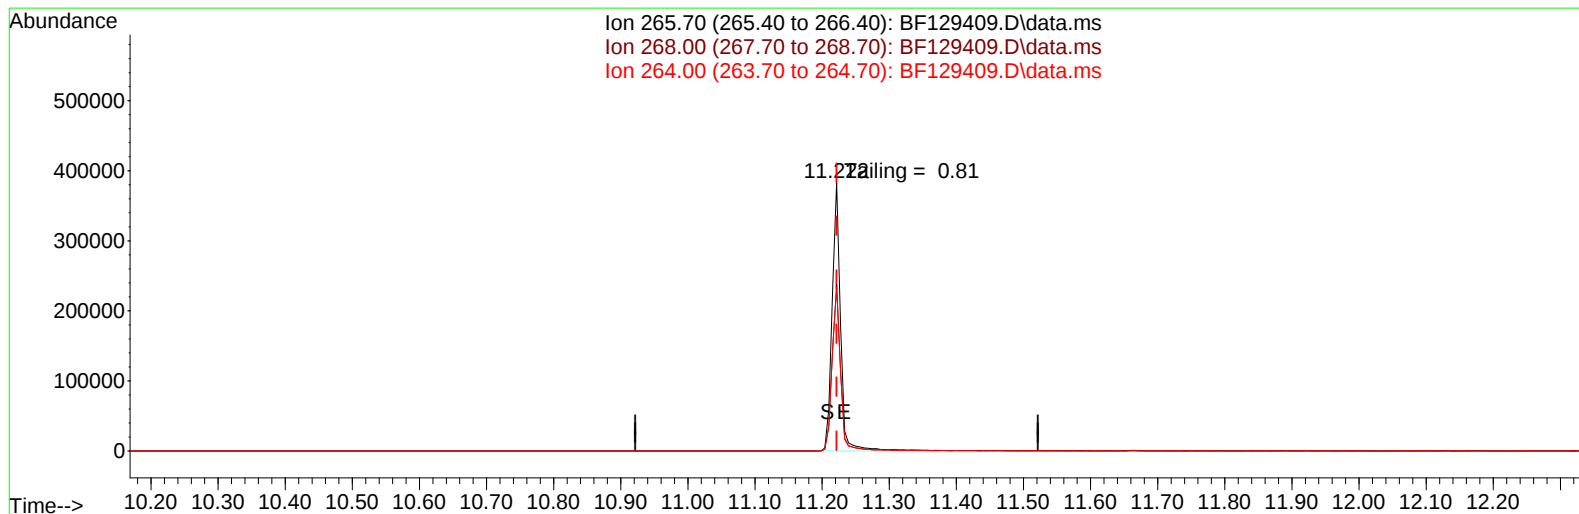

TIC: BF129409.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.000) 520637.09 ng

response 335820

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.03
264.00	61.80	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129409.D
 Acq On : 28 Jul 2022 15:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:38:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

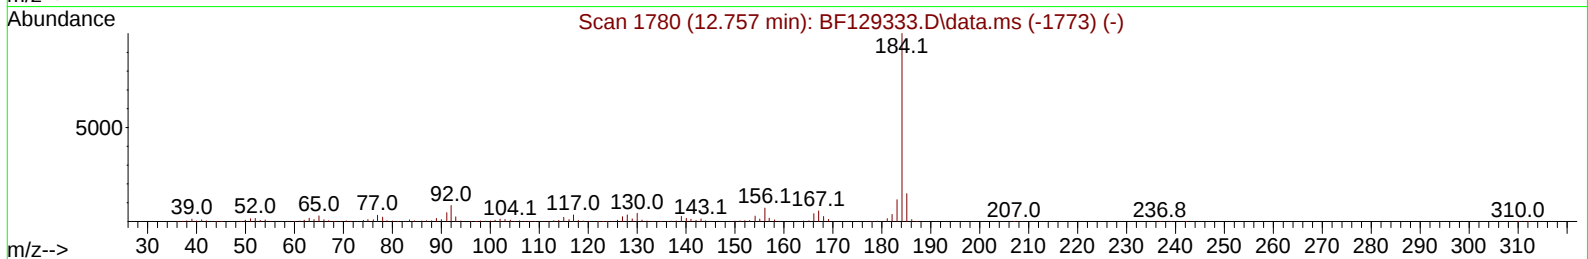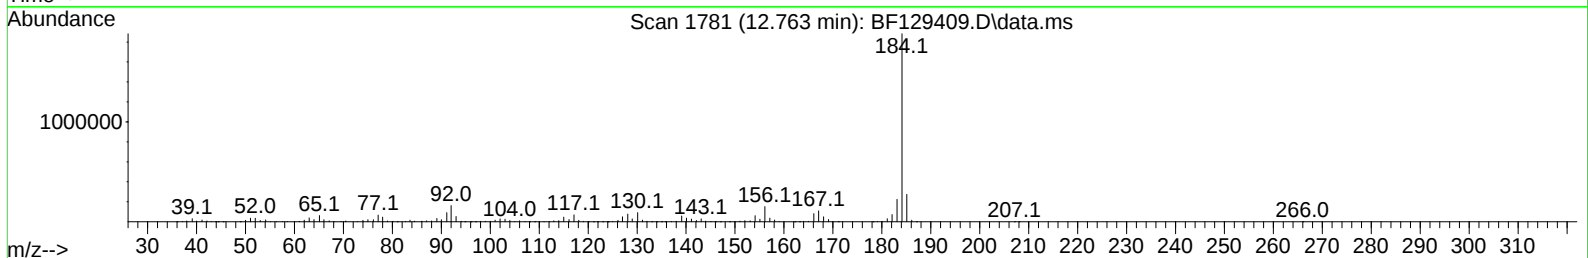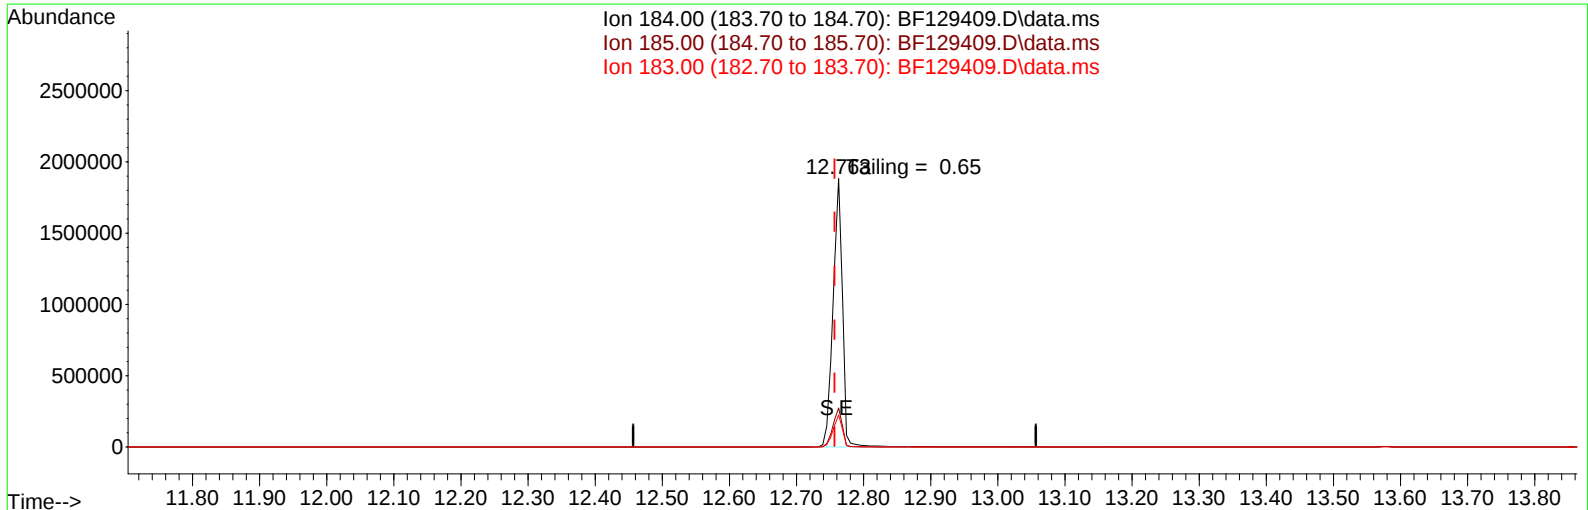

TIC: BF129409.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 117522.83 ng

response 1839243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.54
183.00	11.60	11.94
0.00	0.00	0.00