

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129400.D
 Acq On : 28 Jul 2022 10:20
 Operator : CG\JU
 Sample : PB146497BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146497BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	545	550	553	rBV	5964759	6019903	80.25%	12.915%
2	6.522	714	720	723	rBV	5051000	6128626	81.70%	13.149%
3	6.881	778	781	785	rVB	1565626	1319540	17.59%	2.831%
4	7.451	872	878	881	rBV	4067554	4145239	55.26%	8.893%
5	8.163	994	999	1003	rBV	1885099	1806411	24.08%	3.876%
6	9.245	1176	1183	1186	rBV	7449580	7380367	98.39%	15.834%
7	9.922	1293	1298	1302	rBV	2187770	2038216	27.17%	4.373%
8	10.722	1427	1434	1437	rBV	4540382	4639488	61.85%	9.954%
9	11.416	1548	1552	1555	rBV	2449944	2032548	27.10%	4.361%
10	13.004	1817	1822	1825	rBV	7166389	7501043	100.00%	16.093%
11	14.062	1998	2002	2005	rBV	1902112	1769933	23.60%	3.797%
12	15.551	2249	2255	2267	rBV	1223158	1668118	22.24%	3.579%
13	15.998	2327	2331	2337	rVB	51848	76910	1.03%	0.165%
14	16.515	2415	2419	2427	rVB2	43625	83649	1.12%	0.179%




Sum of corrected areas: 46609991

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129400.D
Acq On : 28 Jul 2022 10:20
Operator : CG\JU
Sample : PB146497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146497BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

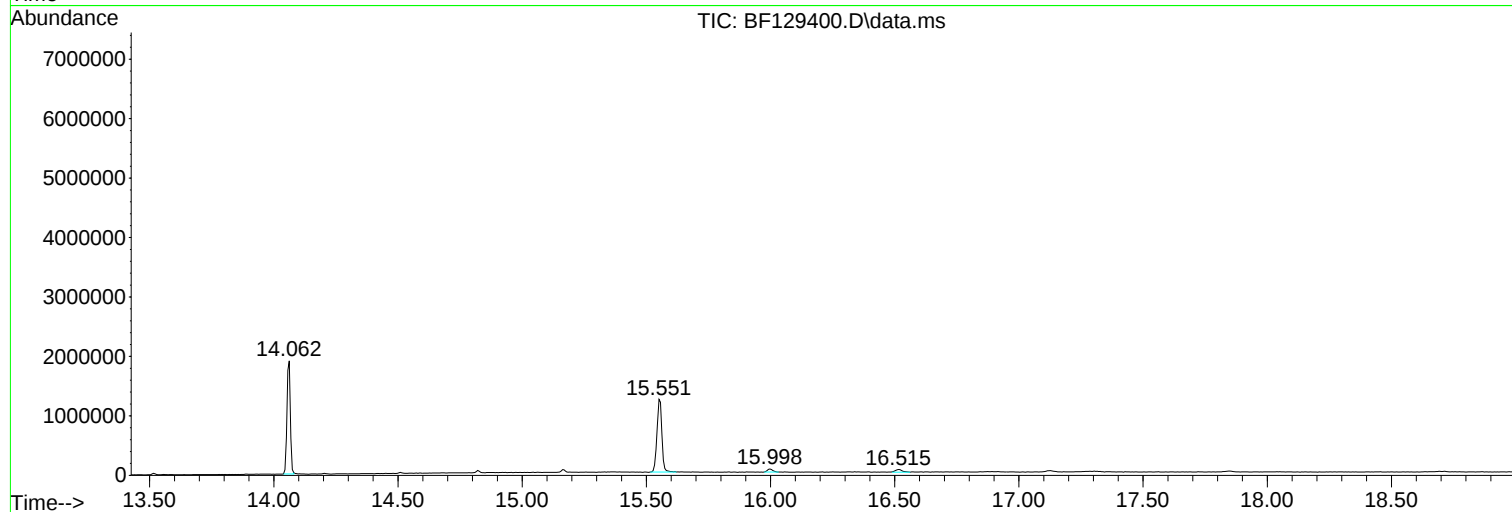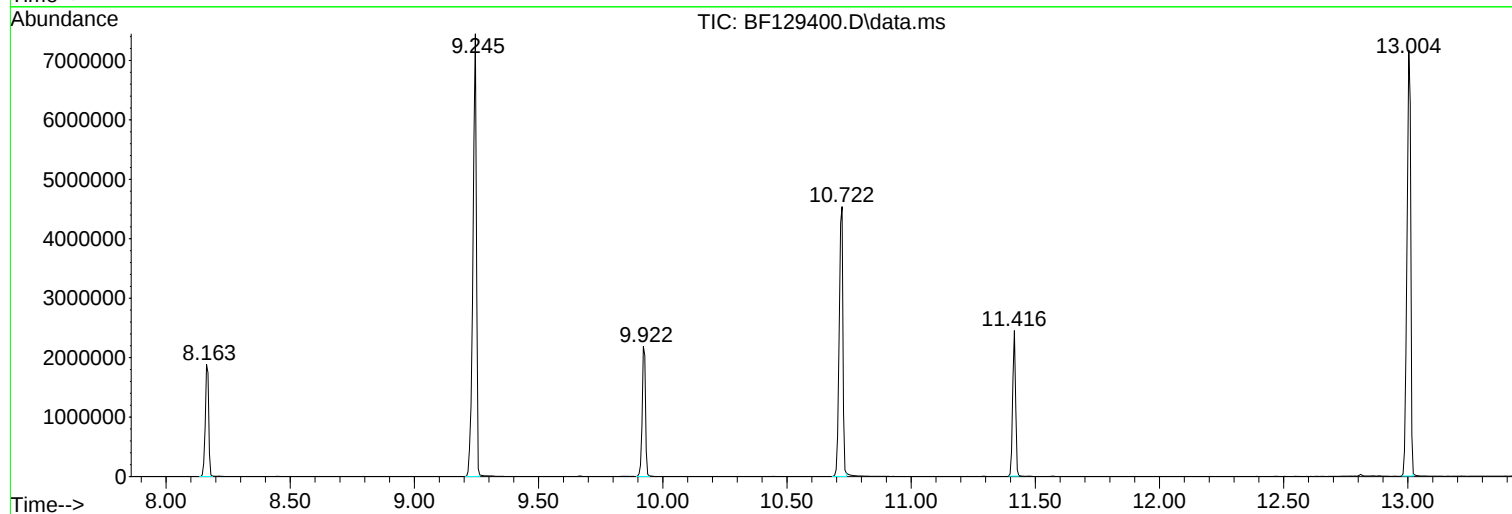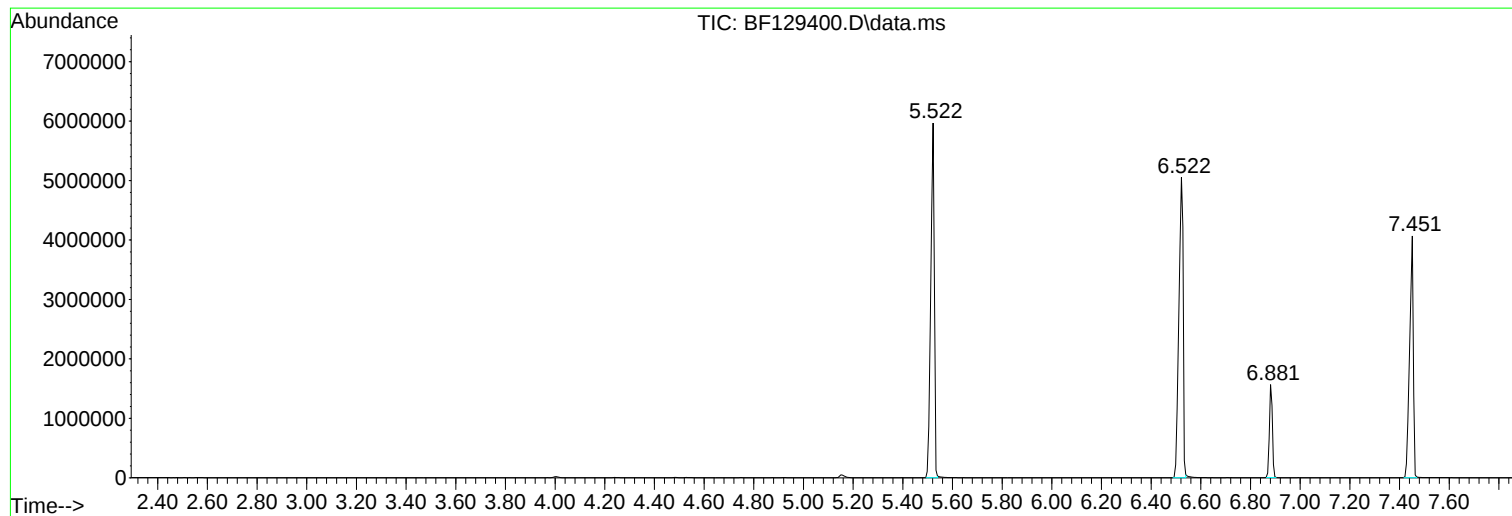

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129400.D
Acq On : 28 Jul 2022 10:20
Operator : CG\JU
Sample : PB146497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146497BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129400.D
Acq On : 28 Jul 2022 10:20
Operator : CG\JU
Sample : PB146497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146497BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------