

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129411.D
 Acq On : 28 Jul 2022 16:22
 Operator : CG\JU
 Sample : PB146473BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146473BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	544	550	553	rBV	6189440	6418173	81.38%	12.949%
2	6.522	714	720	723	rBV	5292243	6602651	83.72%	13.321%
3	6.881	777	781	785	rBV	1761646	1409762	17.88%	2.844%
4	7.451	872	878	881	rBV	4192354	4396024	55.74%	8.869%
5	8.163	994	999	1003	rBV	2115846	1932091	24.50%	3.898%
6	9.245	1176	1183	1186	rBV	7691586	7771723	98.55%	15.680%
7	9.922	1292	1298	1302	rBV	2423505	2203950	27.95%	4.447%
8	10.722	1427	1434	1437	rBV	4811085	4920169	62.39%	9.927%
9	11.416	1544	1552	1555	rBV	2627308	2188534	27.75%	4.416%
10	13.004	1817	1822	1826	rBV	7076835	7886226	100.00%	15.911%
11	14.063	1997	2002	2005	rBV	1835319	1854237	23.51%	3.741%
12	15.551	2249	2255	2266	rBV	1309988	1743509	22.11%	3.518%
13	15.998	2327	2331	2341	rVB	75887	122697	1.56%	0.248%
14	16.515	2414	2419	2426	rVB2	63696	114126	1.45%	0.230%




Sum of corrected areas: 49563872

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129411.D
Acq On : 28 Jul 2022 16:22
Operator : CG\JU
Sample : PB146473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

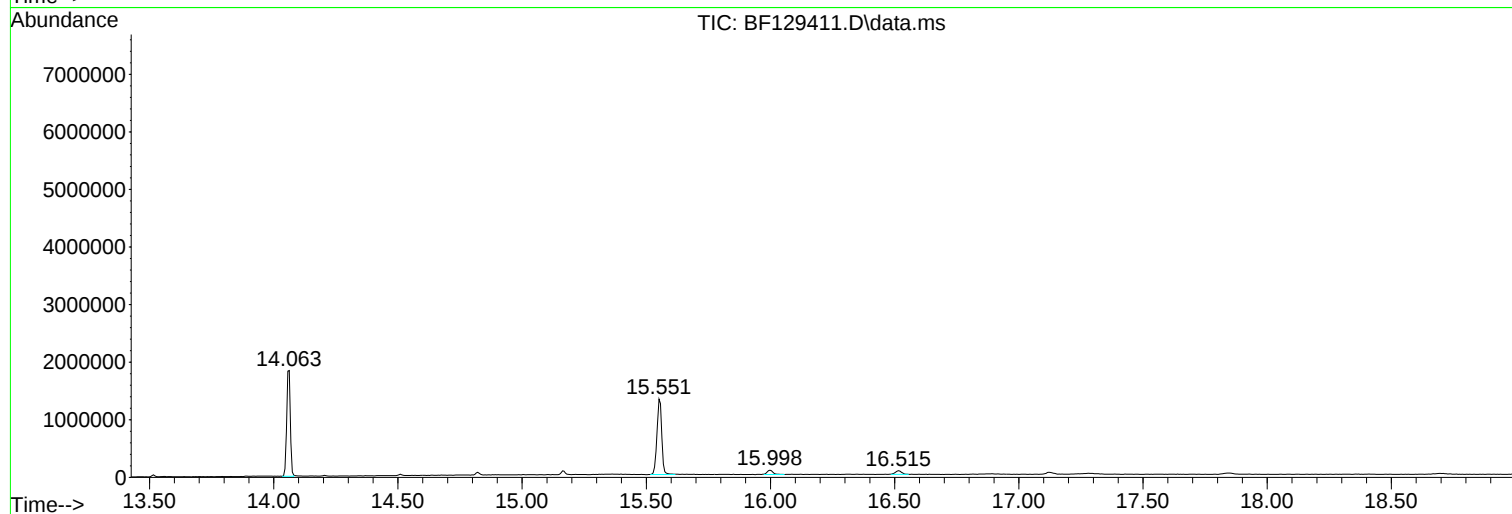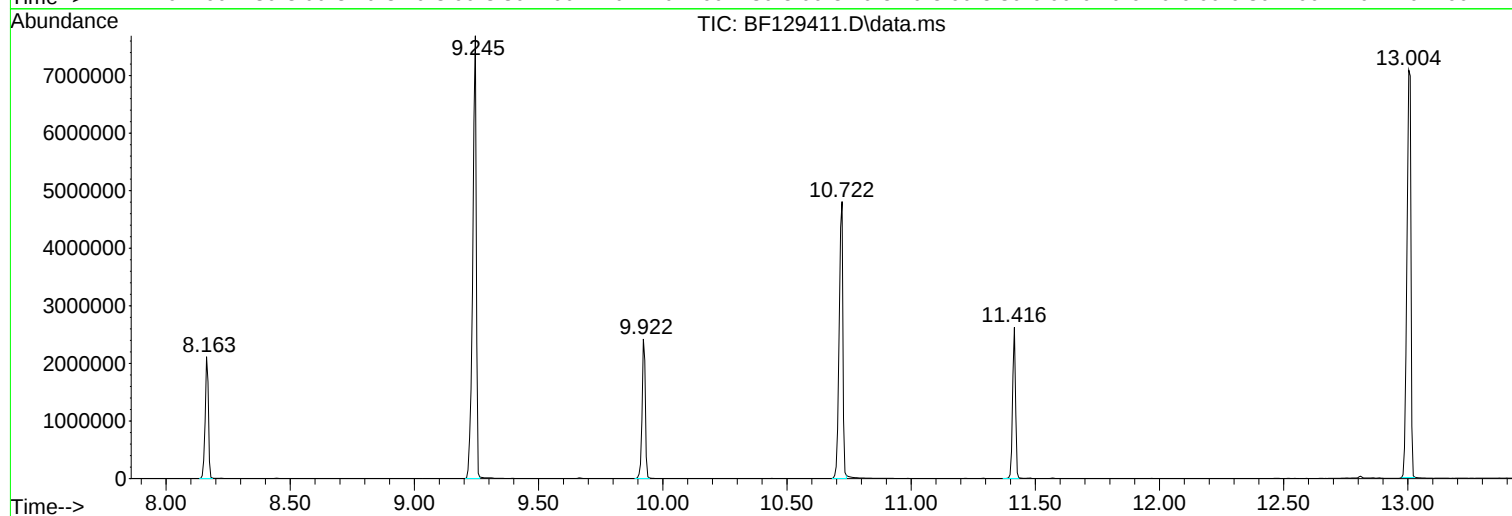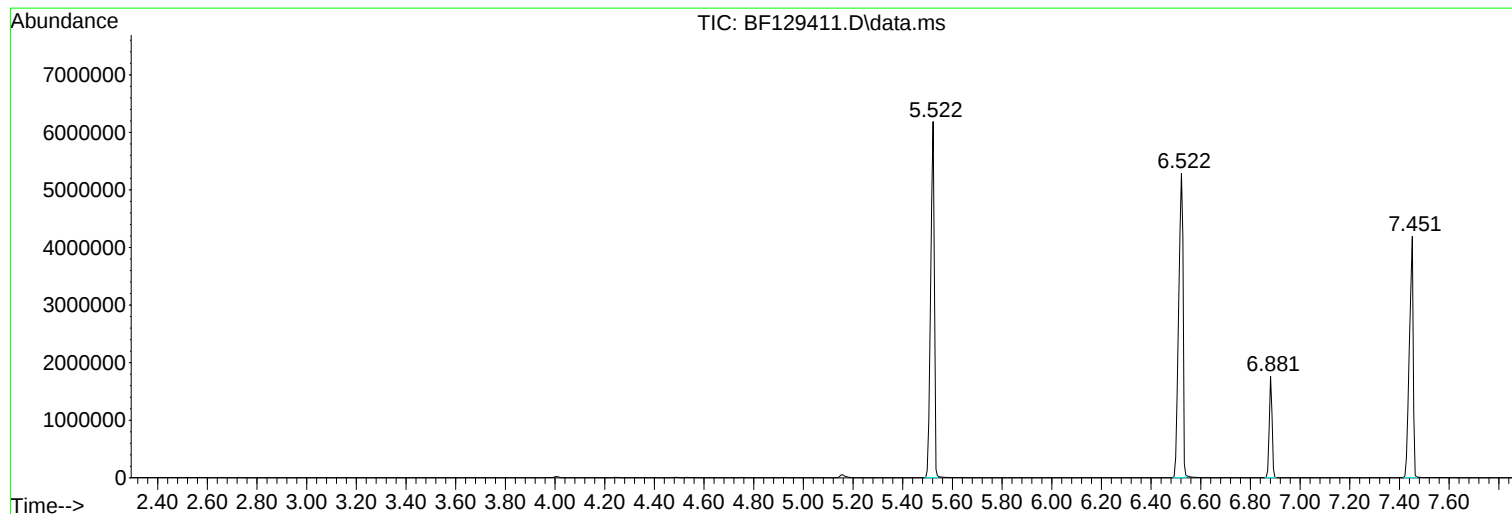

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129411.D
Acq On : 28 Jul 2022 16:22
Operator : CG\JU
Sample : PB146473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129411.D
Acq On : 28 Jul 2022 16:22
Operator : CG\JU
Sample : PB146473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------