

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129418.D
 Acq On : 28 Jul 2022 20:18
 Operator : CG\JU
 Sample : N3894-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RVE-35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	478	481	495	rVB	81884	107473	2.18%	0.287%
2	5.510	544	548	551	rBV	3983738	3687534	74.95%	9.832%
3	6.522	714	720	723	rBV	3532266	3794324	77.12%	10.117%
4	6.881	777	781	785	rBV	1550549	1264193	25.70%	3.371%
5	7.445	872	877	880	rBV	2734911	2640166	53.67%	7.039%
6	8.163	995	999	1002	rBV	1918169	1707759	34.71%	4.553%
7	9.239	1177	1182	1185	rBV	5415609	4919711	100.00%	13.117%
8	9.922	1292	1298	1302	rBV	2274480	1896913	38.56%	5.058%
9	10.716	1429	1433	1436	rBV	3030969	2558554	52.01%	6.822%
10	10.816	1447	1450	1459	rVB3	55683	92823	1.89%	0.247%
11	11.410	1548	1551	1554	rBV	1750353	1630218	33.14%	4.347%
12	11.433	1554	1555	1558	rVB	126916	88533	1.80%	0.236%
13	11.916	1631	1637	1638	rBV	43839	51519	1.05%	0.137%
14	11.939	1638	1641	1644	rVB2	58576	72574	1.48%	0.194%
15	12.022	1652	1655	1658	rBV2	52467	53841	1.09%	0.144%
16	12.098	1665	1668	1671	rBV	62896	54935	1.12%	0.146%
17	12.233	1689	1691	1698	rVB4	44309	51871	1.05%	0.138%
18	12.463	1727	1730	1732	rBV	54939	56616	1.15%	0.151%
19	12.486	1732	1734	1738	rVB2	72838	70416	1.43%	0.188%
20	12.627	1755	1758	1762	rVB	293078	239123	4.86%	0.638%
21	12.857	1791	1797	1800	rBV	319844	312498	6.35%	0.833%
22	12.998	1817	1821	1824	rBV	3906543	3304316	67.16%	8.810%
23	13.068	1830	1833	1840	rBV5	29043	51611	1.05%	0.138%
24	13.216	1855	1858	1862	rBV	88672	89746	1.82%	0.239%
25	13.557	1913	1916	1919	rBV2	85770	89539	1.82%	0.239%
26	13.692	1934	1939	1945	rBV	39575	63510	1.29%	0.169%
27	13.904	1969	1975	1986	rBV2	248095	624430	12.69%	1.665%
28	14.057	1997	2001	2004	rBV	1175770	1110229	22.57%	2.960%
29	14.080	2004	2005	2013	rVB	116702	113446	2.31%	0.302%
30	14.204	2023	2026	2029	rBV	80523	72160	1.47%	0.192%
31	14.510	2075	2078	2081	rBV	143605	131246	2.67%	0.350%
32	14.821	2128	2131	2135	rVB	60401	63998	1.30%	0.171%
33	14.968	2153	2156	2161	rVB	83808	83059	1.69%	0.221%
34	15.110	2176	2180	2183	rBV2	104717	152105	3.09%	0.406%
35	15.162	2186	2189	2194	rVB	198593	212759	4.32%	0.567%
36	15.221	2196	2199	2201	rBV3	49388	69331	1.41%	0.185%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129418.D
Acq On : 28 Jul 2022 20:18
Operator : CG\JU
Sample : N3894-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-35

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.421	2230	2233	2240	rVB	68647	90341	1.84%	0.241%
38	15.486	2240	2244	2249	rVB	78296	105253	2.14%	0.281%
39	15.551	2250	2255	2266	rVV	900427	1159974	23.58%	3.093%
40	15.762	2288	2291	2295	rVB2	89486	111841	2.27%	0.298%
41	15.992	2326	2330	2337	rVB	207164	331863	6.75%	0.885%
42	16.127	2349	2353	2366	rVB2	103230	224072	4.55%	0.597%
43	16.821	2466	2471	2478	rVB4	68585	129320	2.63%	0.345%
44	17.221	2531	2539	2547	rBV2	1509114	3119788	63.41%	8.318%
45	17.562	2592	2597	2605	rVB4	162877	352051	7.16%	0.939%
46	18.068	2679	2683	2692	rVB7	134102	297746	6.05%	0.794%




Sum of corrected areas: 37505328

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129418.D
Acq On : 28 Jul 2022 20:18
Operator : CG\JU
Sample : N3894-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

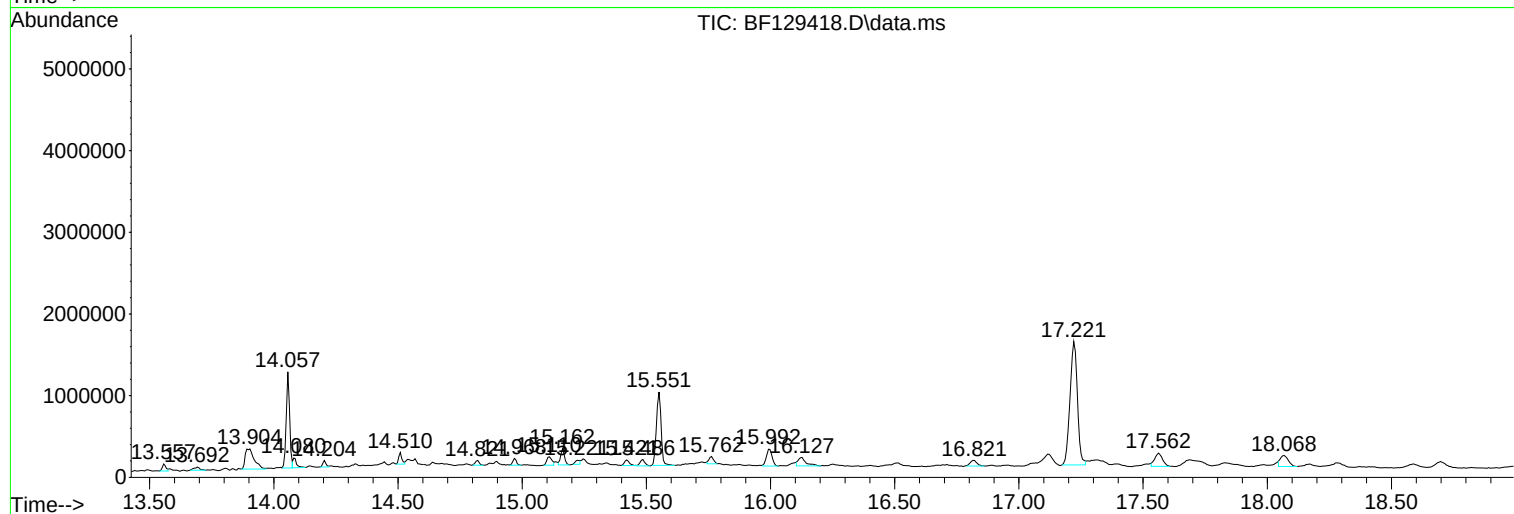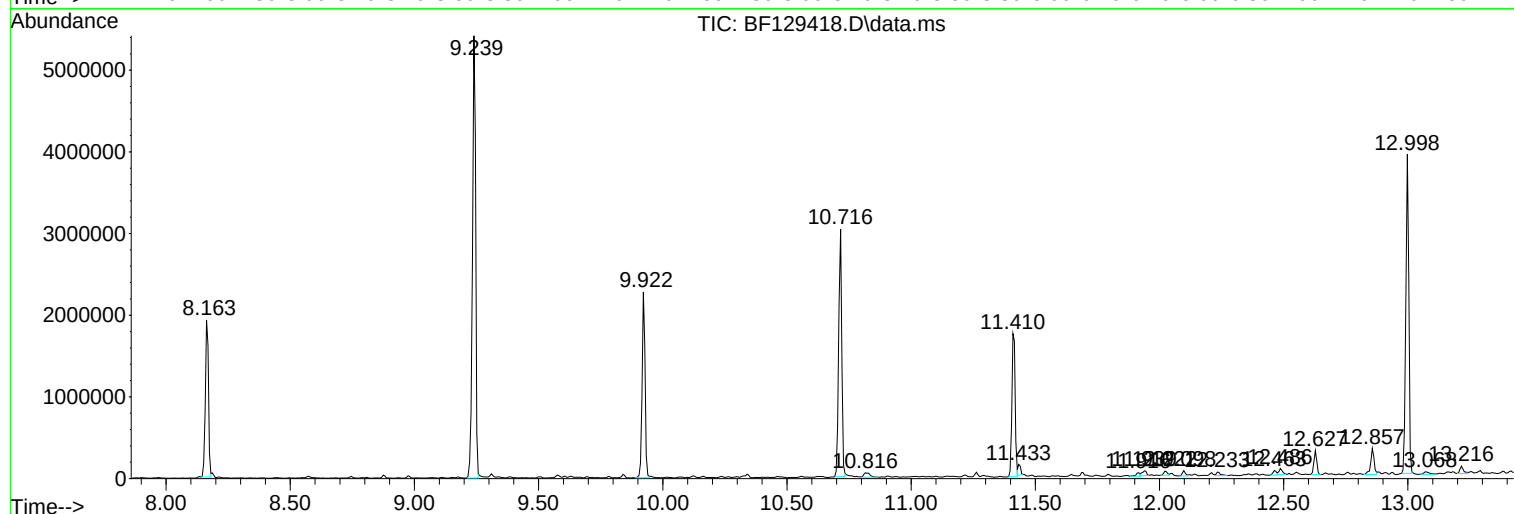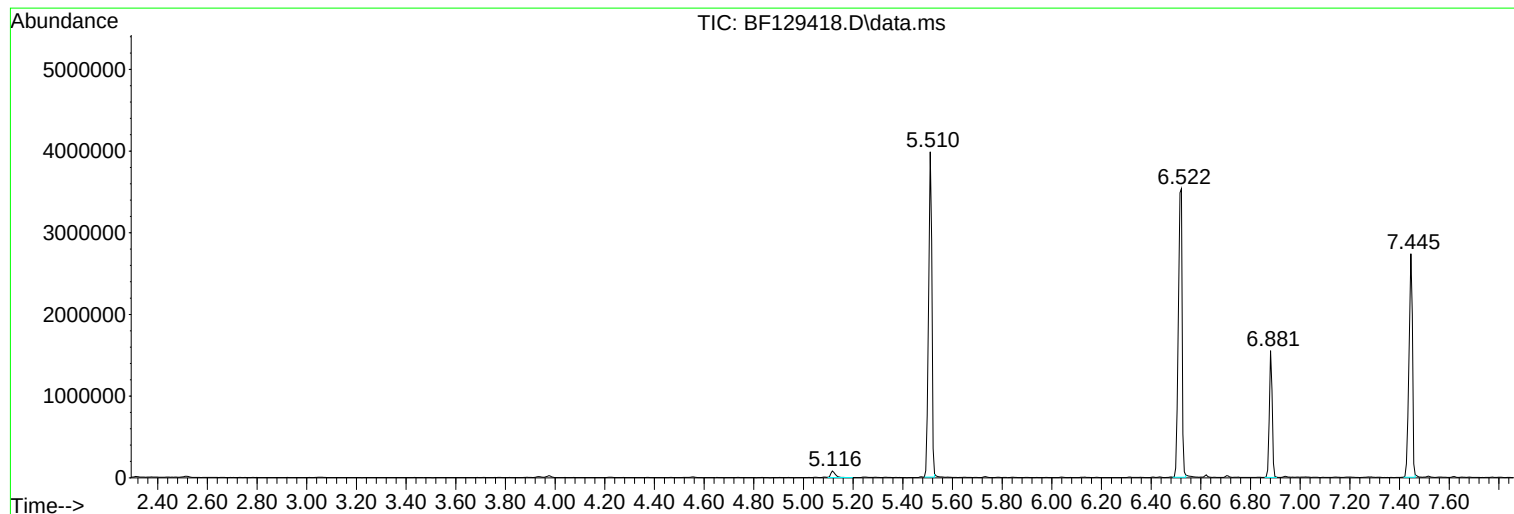

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129418.D
Acq On : 28 Jul 2022 20:18
Operator : CG\JU
Sample : N3894-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129418.D
Acq On : 28 Jul 2022 20:18
Operator : CG\JU
Sample : N3894-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------