

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129430.D
 Acq On : 29 Jul 2022 02:53
 Operator : CG\JU
 Sample : N3923-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-072722

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	279	284	292	rVB	17248	23878	1.76%	0.207%
2	5.510	544	548	560	rBV	1083835	960890	70.71%	8.339%
3	6.522	716	720	731	rBV	951470	926709	68.20%	8.042%
4	6.887	778	782	785	rBV	1472269	1143893	84.18%	9.927%
5	7.445	873	877	880	rBV	700624	528048	38.86%	4.583%
6	8.169	996	1000	1004	rBV	1751425	1358906	100.00%	11.793%
7	9.239	1179	1182	1186	rBV	1091109	924250	68.01%	8.021%
8	9.928	1295	1299	1303	rBV	1653358	1261642	92.84%	10.949%
9	10.716	1430	1433	1442	rBV	537992	494234	36.37%	4.289%
10	10.834	1448	1453	1459	rVB7	15935	27926	2.06%	0.242%
11	11.416	1549	1552	1556	rBV	1259243	1177136	86.62%	10.216%
12	11.651	1590	1592	1596	rBV5	15779	17424	1.28%	0.151%
13	12.345	1708	1710	1714	rBV4	36599	35684	2.63%	0.310%
14	12.633	1756	1759	1761	rBV	89921	83052	6.11%	0.721%
15	12.863	1796	1798	1802	rBV	143999	140724	10.36%	1.221%
16	13.004	1818	1822	1825	rBV	936526	789165	58.07%	6.849%
17	14.069	1999	2003	2006	rBV	958281	921559	67.82%	7.998%
18	15.568	2254	2258	2262	rVB	589640	707911	52.09%	6.143%




Sum of corrected areas: 11523031

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129430.D
Acq On : 29 Jul 2022 02:53
Operator : CG\JU
Sample : N3923-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-072722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

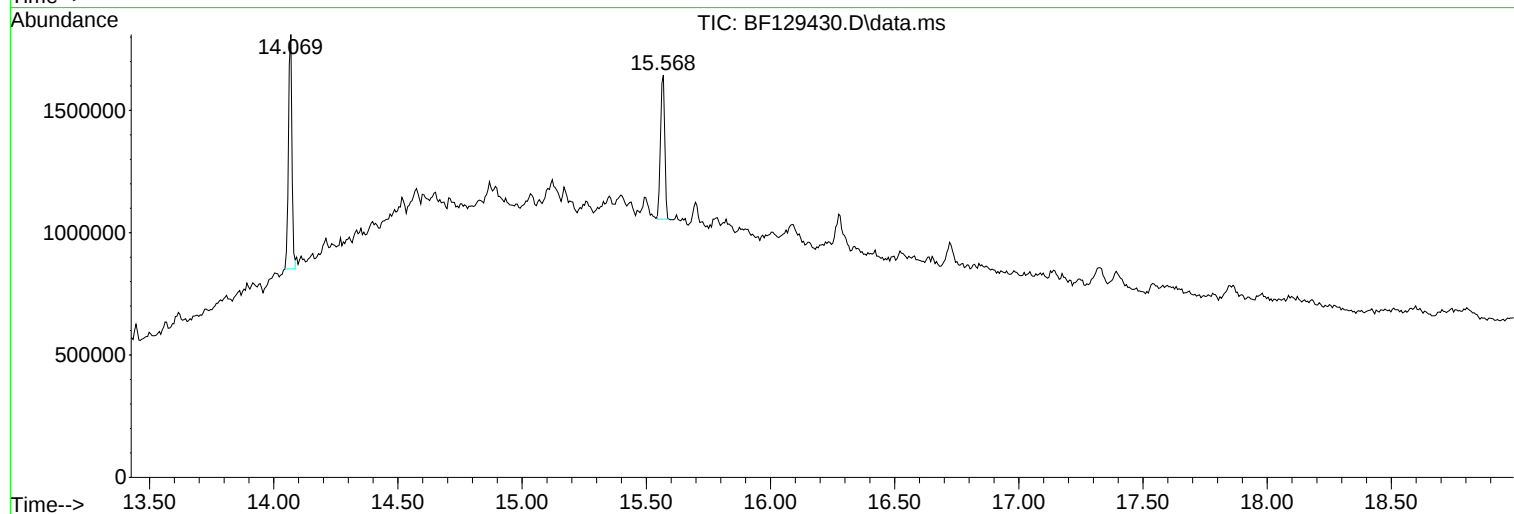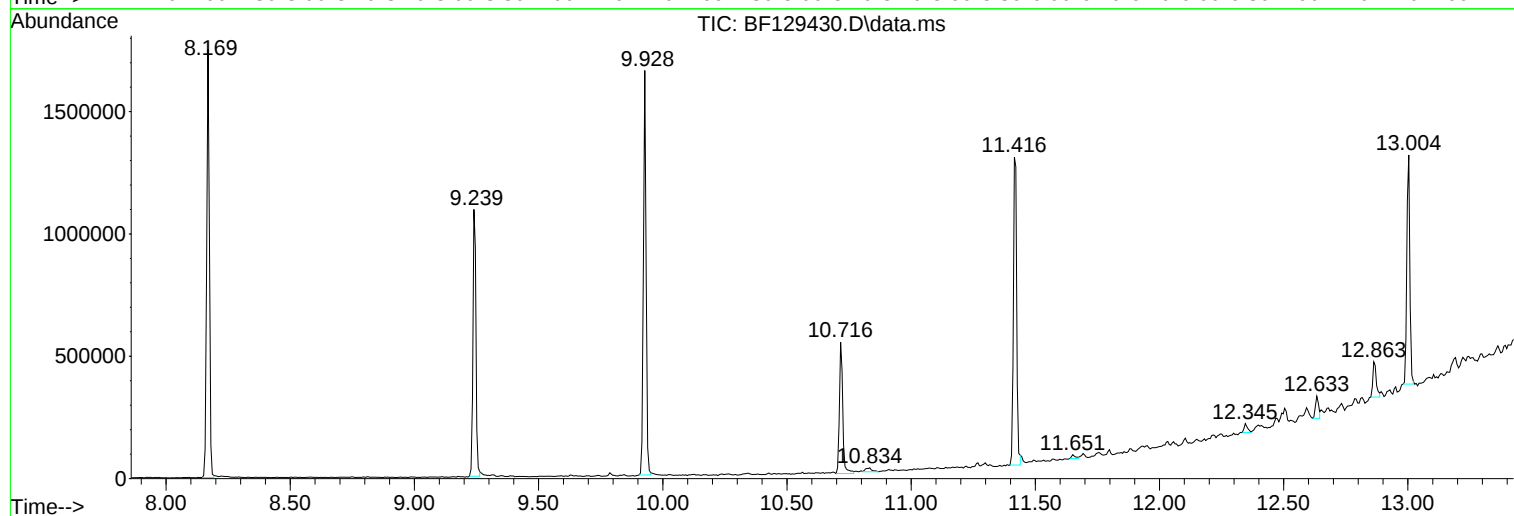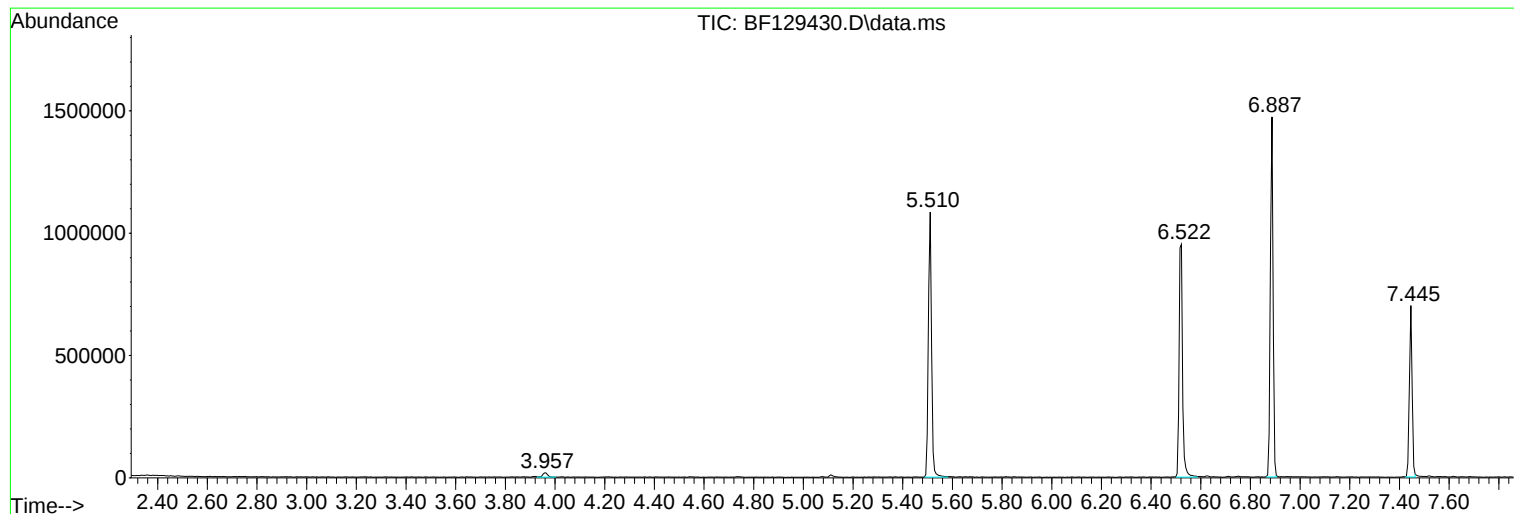

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129430.D
Acq On : 29 Jul 2022 02:53
Operator : CG\JU
Sample : N3923-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-072722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129430.D
Acq On : 29 Jul 2022 02:53
Operator : CG\JU
Sample : N3923-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-072722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------