


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
 Data File : BF129409.D
 Acq On : 28 Jul 2022 15:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 04:30:50 2022

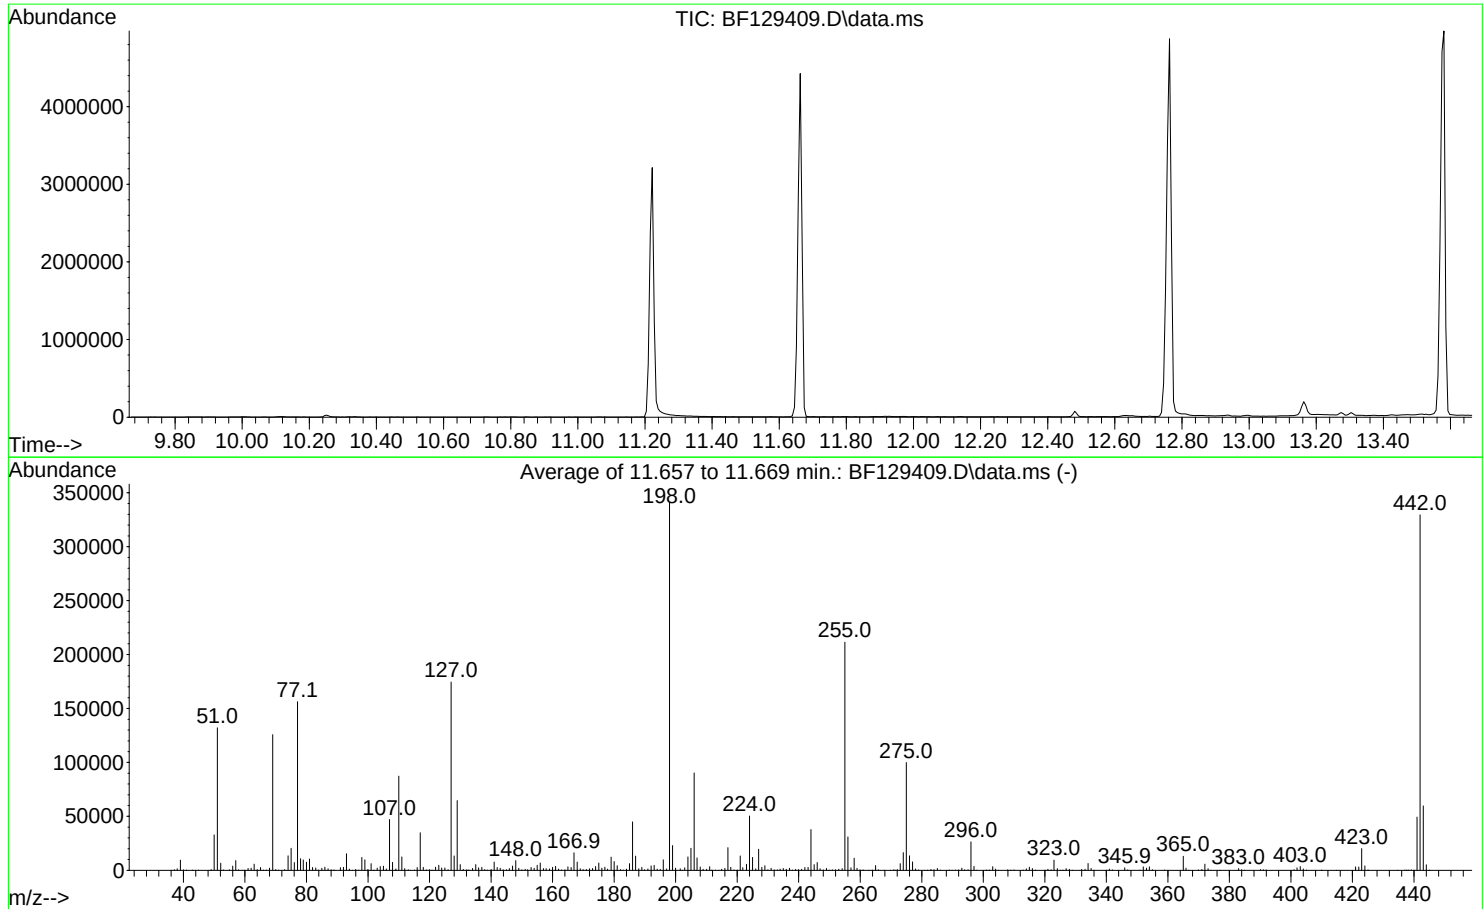




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	132104	PASS
68	69	0.00	2	1.6	2060	PASS
69	198	0.00	100	36.9	125704	PASS
70	69	0.00	2	0.6	718	PASS
127	198	10	80	51.2	174587	PASS
197	198	0.00	2	0.4	1306	PASS
198	198	100	100	100.0	341013	PASS
199	198	5	9	6.7	22861	PASS
275	198	10	60	29.3	99931	PASS
365	198	1	100	3.8	13033	PASS
441	198	0.01	100	14.5	49339	PASS
442	442	50	100	100.0	329579	PASS
443	442	15	24	18.1	59656	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129409.D
Acq On : 28 Jul 2022 15:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:38:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

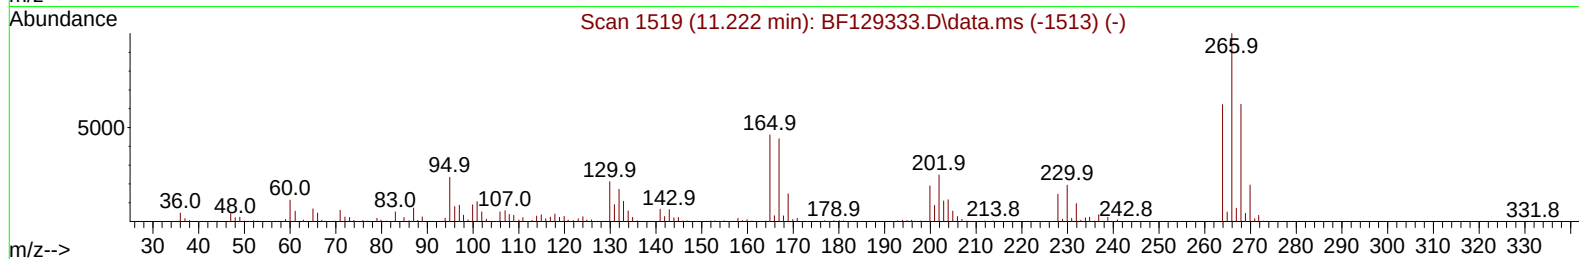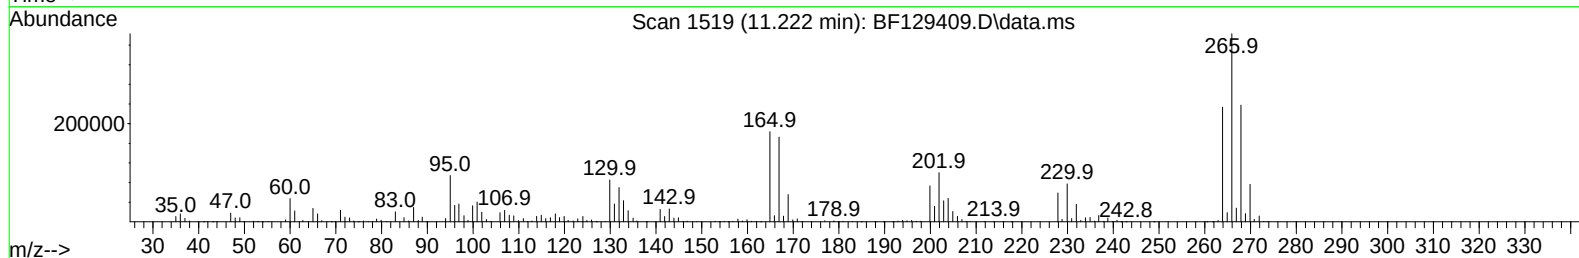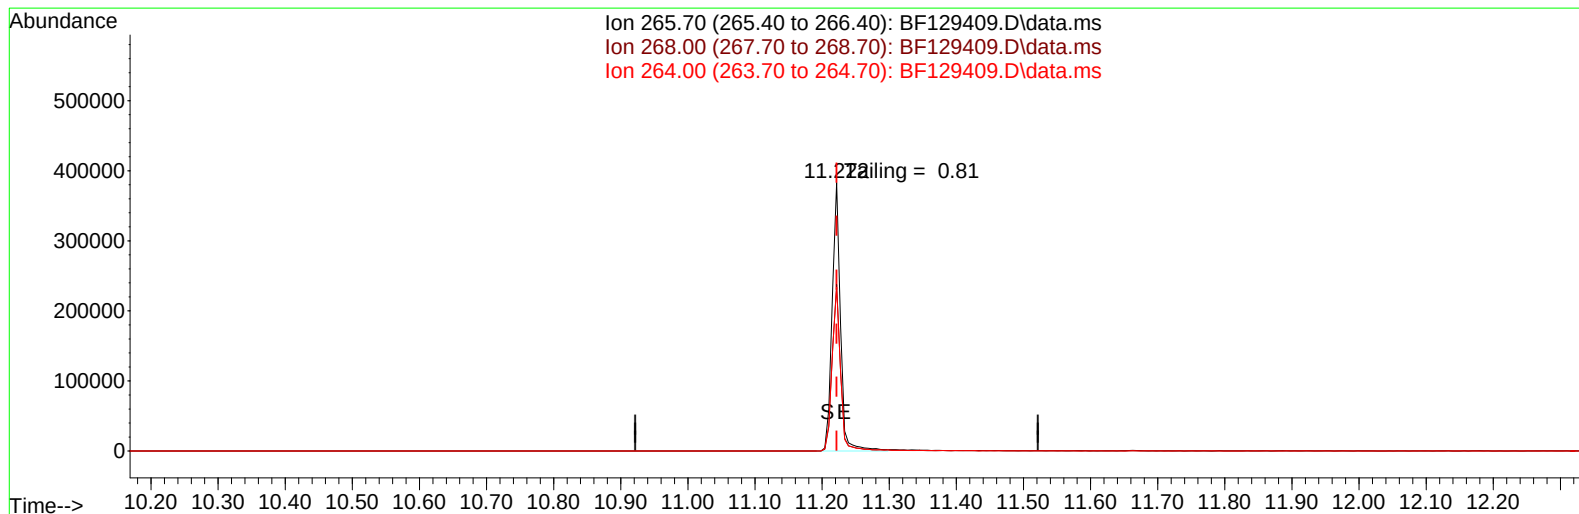

TIC: BF129409.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 520637.09 ng




response 335820

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.03
264.00	61.80	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072822\
Data File : BF129409.D
Acq On : 28 Jul 2022 15:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:38:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

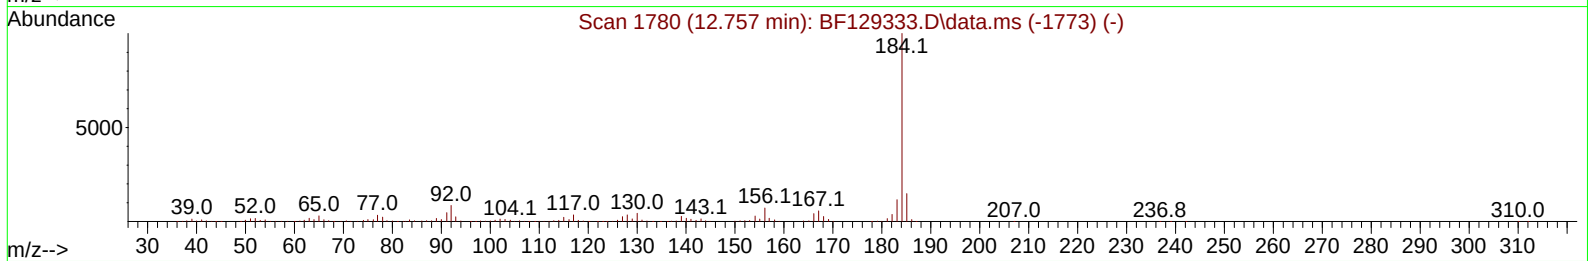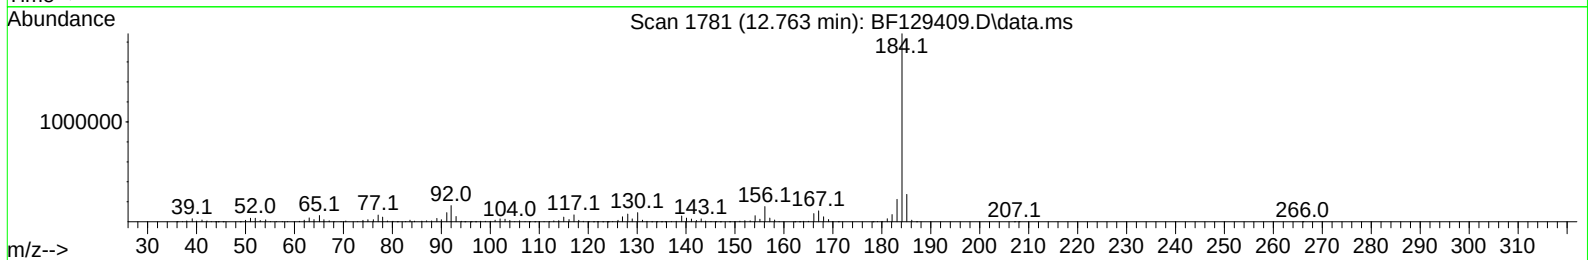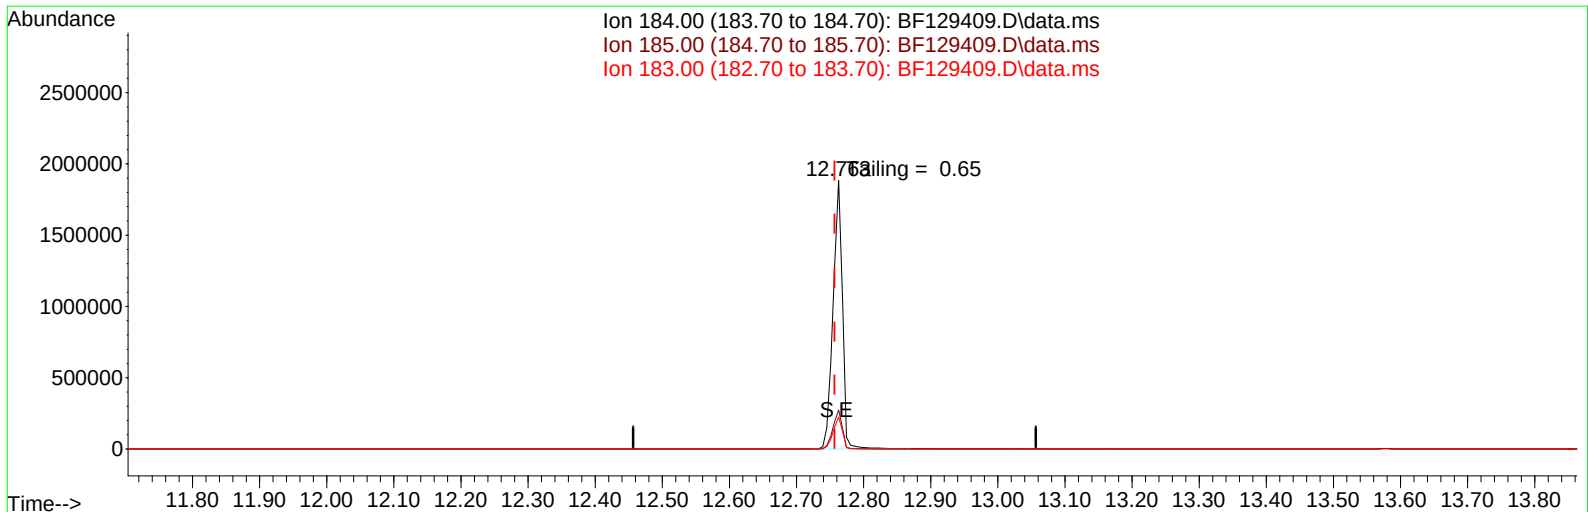

TIC: BF129409.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 117522.83 ng

response 1839243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.54
183.00	11.60	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2022	BNA_F	<u>BF129409.D</u>
Compound Name	Response	Retention Time
DDT	906631	13.58
DDD	10162	13.274
DDE	1400	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11562	918193	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP