


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072916\
 Data File : BF089365.D
 Acq On : 28 Jul 2016 16:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

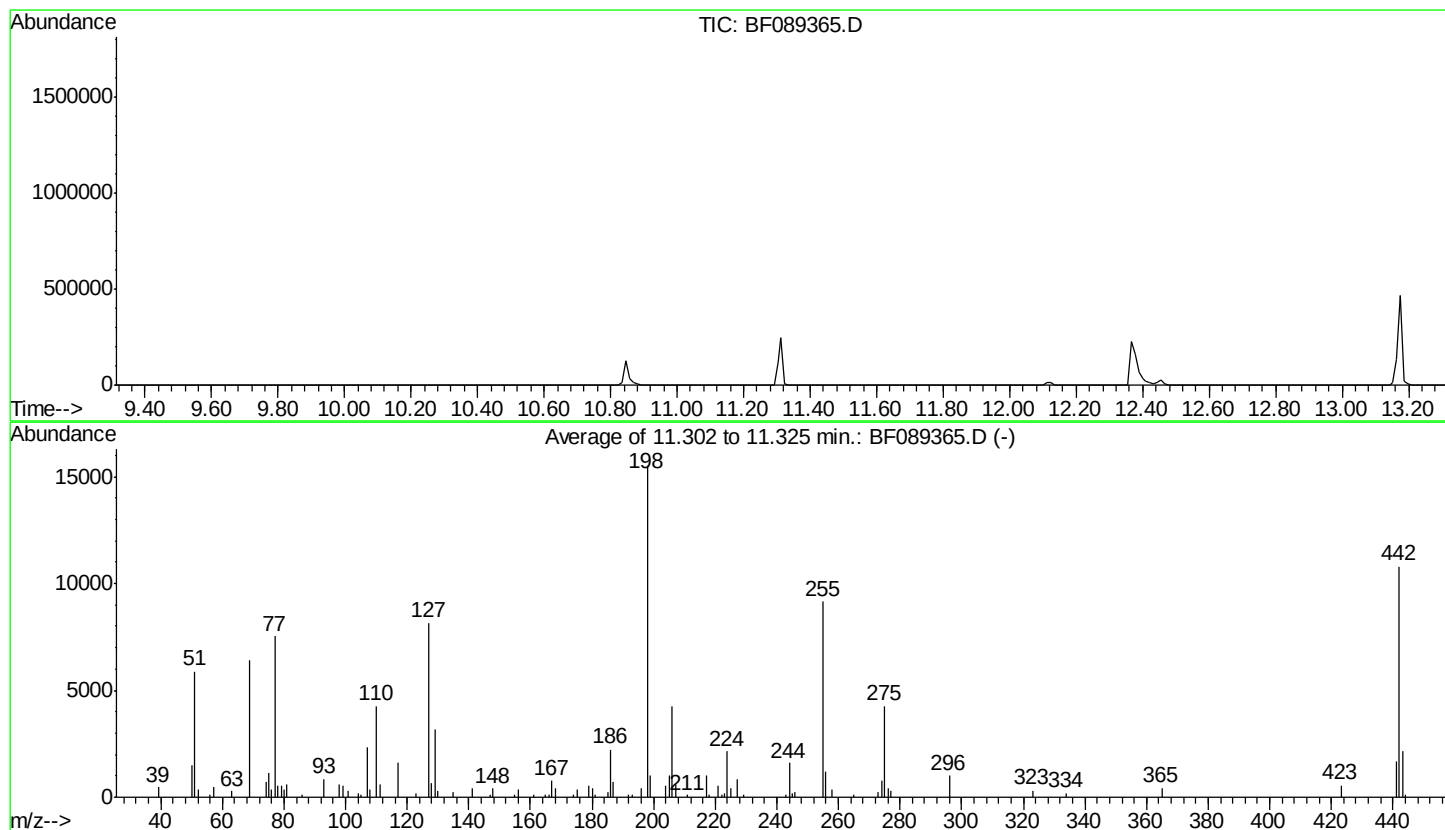

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	5876	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.5	6434	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	8176	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15516	PASS
199	198	5	9	6.6	1020	PASS
275	198	10	60	27.5	4270	PASS
365	198	1	100	2.8	431	PASS
441	442	0.01	24	15.7	1695	PASS
442	198	50	100	69.5	10788	PASS
443	442	15	24	20.2	2182	PASS