
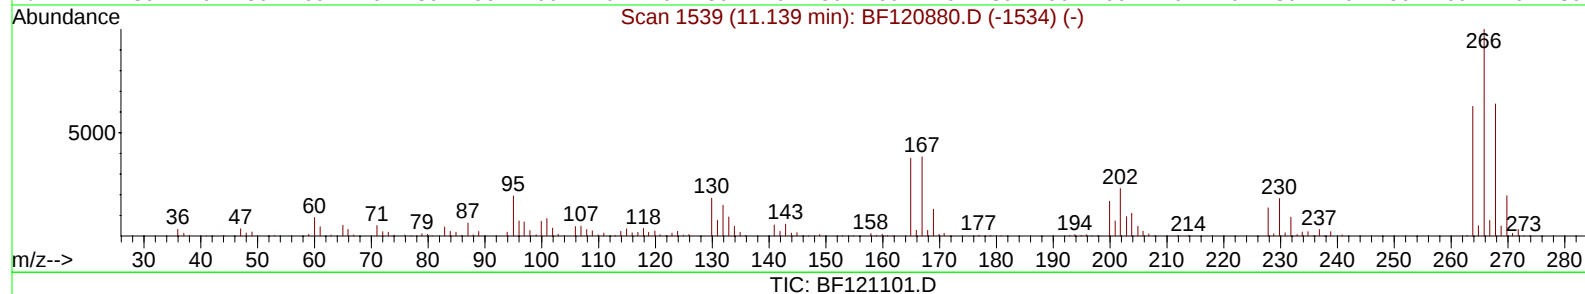
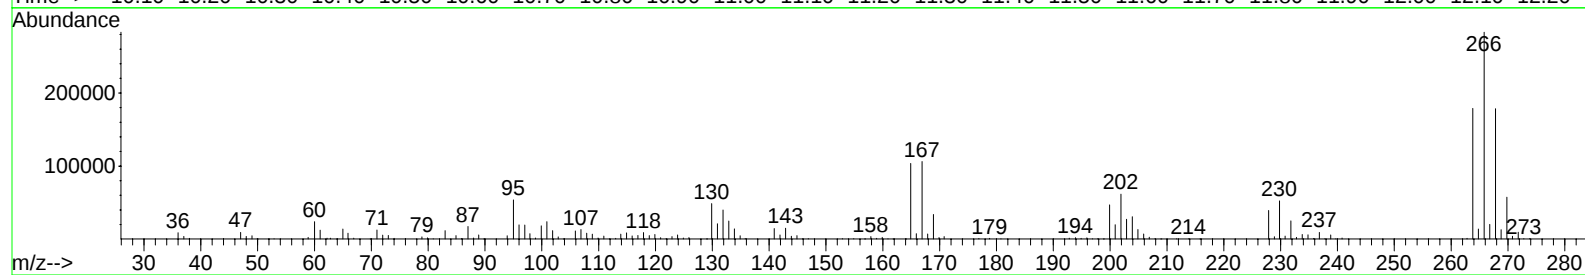


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072920\
 Data File : BF121101.D
 Acq On : 29 Jul 2020 14:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 18:52:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

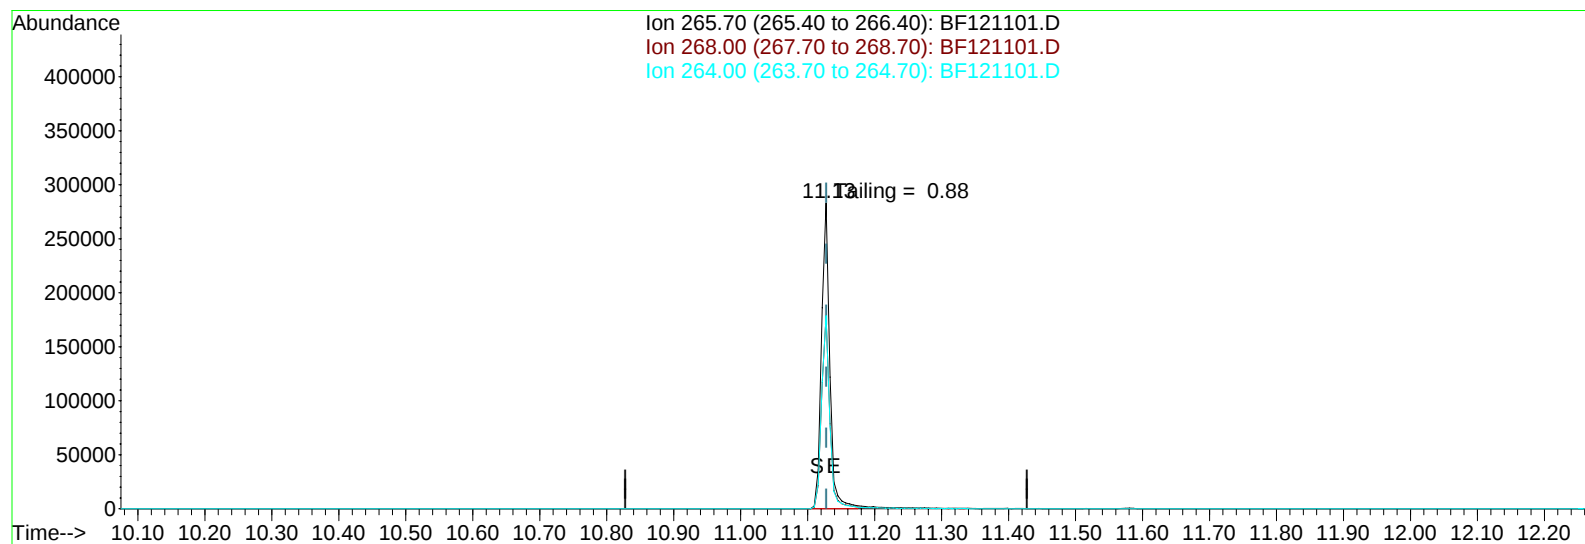

(70) Pentachlorophenol (C)




11.128min (+0.000) 98600.34ng

response 250022

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.07
264.00	63.00	63.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072920\
 Data File : BF121101.D
 Acq On : 29 Jul 2020 14:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 18:52:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

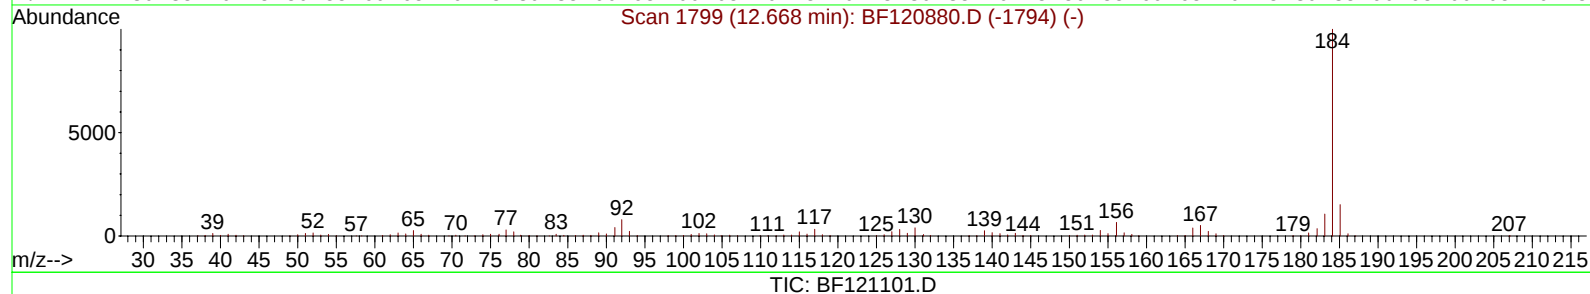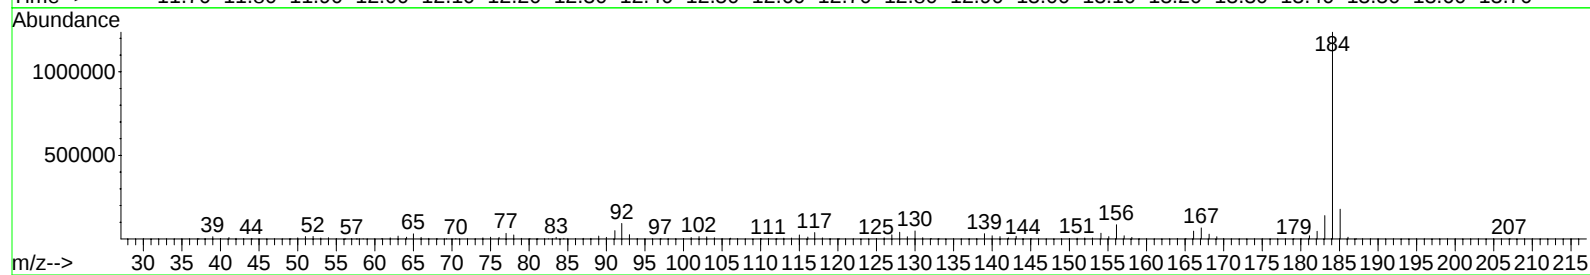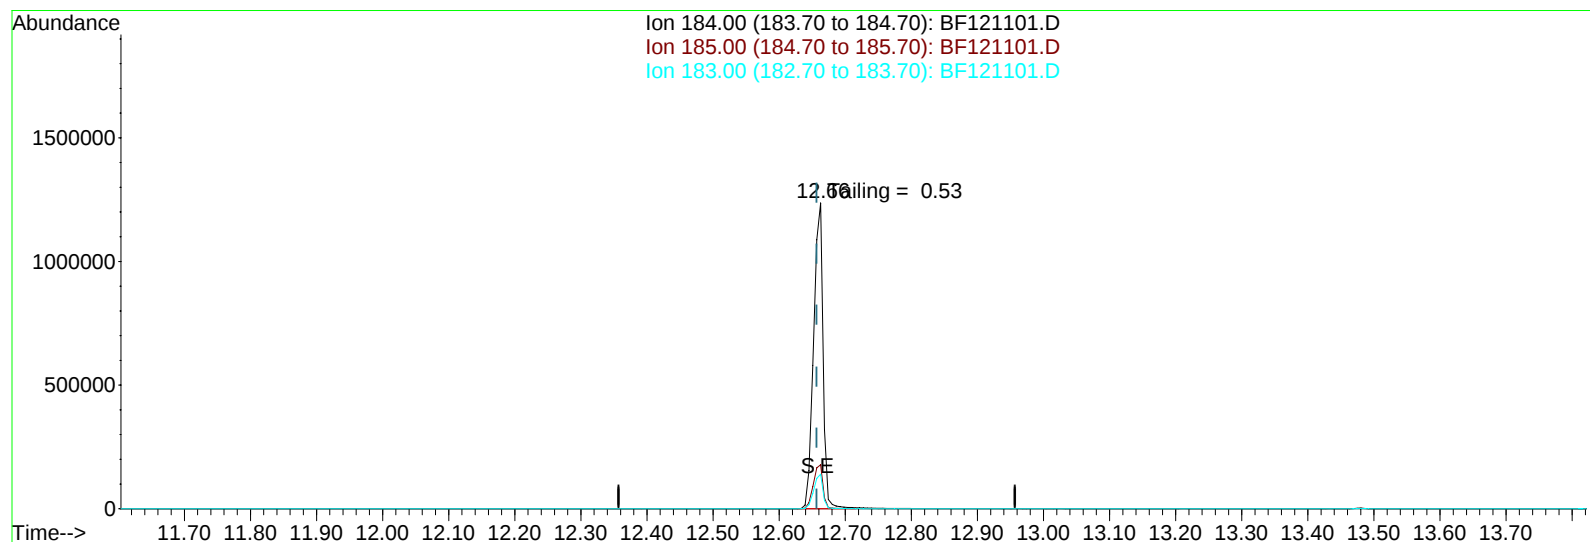

(77) Benzidine

12.663min (+0.006) 141435.18ng

response 1242007

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.39
183.00	11.20	11.31
0.00	0.00	0.00