

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072920\
 Data File : BF121099.D
 Acq On : 29 Jul 2020 13:37
 Operator : JU/CG
 Sample : PB130545BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130545BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.857	295	301	308	rVB	37504	50356	1.15%	0.179%
2	5.016	495	498	506	rBV	36649	49043	1.12%	0.175%
3	5.422	563	567	571	rBV	2603389	2439635	55.94%	8.681%
4	6.434	734	739	742	rBV	2347700	2385593	54.70%	8.489%
5	6.798	798	801	805	rBV	1060211	900880	20.66%	3.206%
6	6.957	824	828	831	rBV	3224086	2995081	68.67%	10.658%
7	7.363	892	897	900	rBV	2325631	2385112	54.69%	8.487%
8	8.081	1015	1019	1023	rBV	1220191	1135132	26.03%	4.039%
9	9.157	1197	1202	1206	rBV	3902091	4238667	97.19%	15.083%
10	9.833	1312	1317	1321	rBV	1436327	1293016	29.65%	4.601%
11	10.622	1446	1451	1465	rBV	1989164	1876097	43.02%	6.676%
12	11.322	1565	1570	1577	rBV	1356708	1353904	31.04%	4.818%
13	12.910	1835	1840	1843	rBV	4058323	4361310	100.00%	15.519%
14	13.957	2014	2018	2021	rBV	1319711	1272276	29.17%	4.527%
15	15.398	2258	2263	2273	rBV2	1015325	1268428	29.08%	4.514%
16	15.851	2336	2340	2346	rVB2	35575	49955	1.15%	0.178%
17	16.339	2418	2423	2431	rVB2	26216	47690	1.09%	0.170%


Sum of corrected areas: 28102175

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072920\
Data File : BF121099.D
Acq On : 29 Jul 2020 13:37
Operator : JU/CG
Sample : PB130545BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130545BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

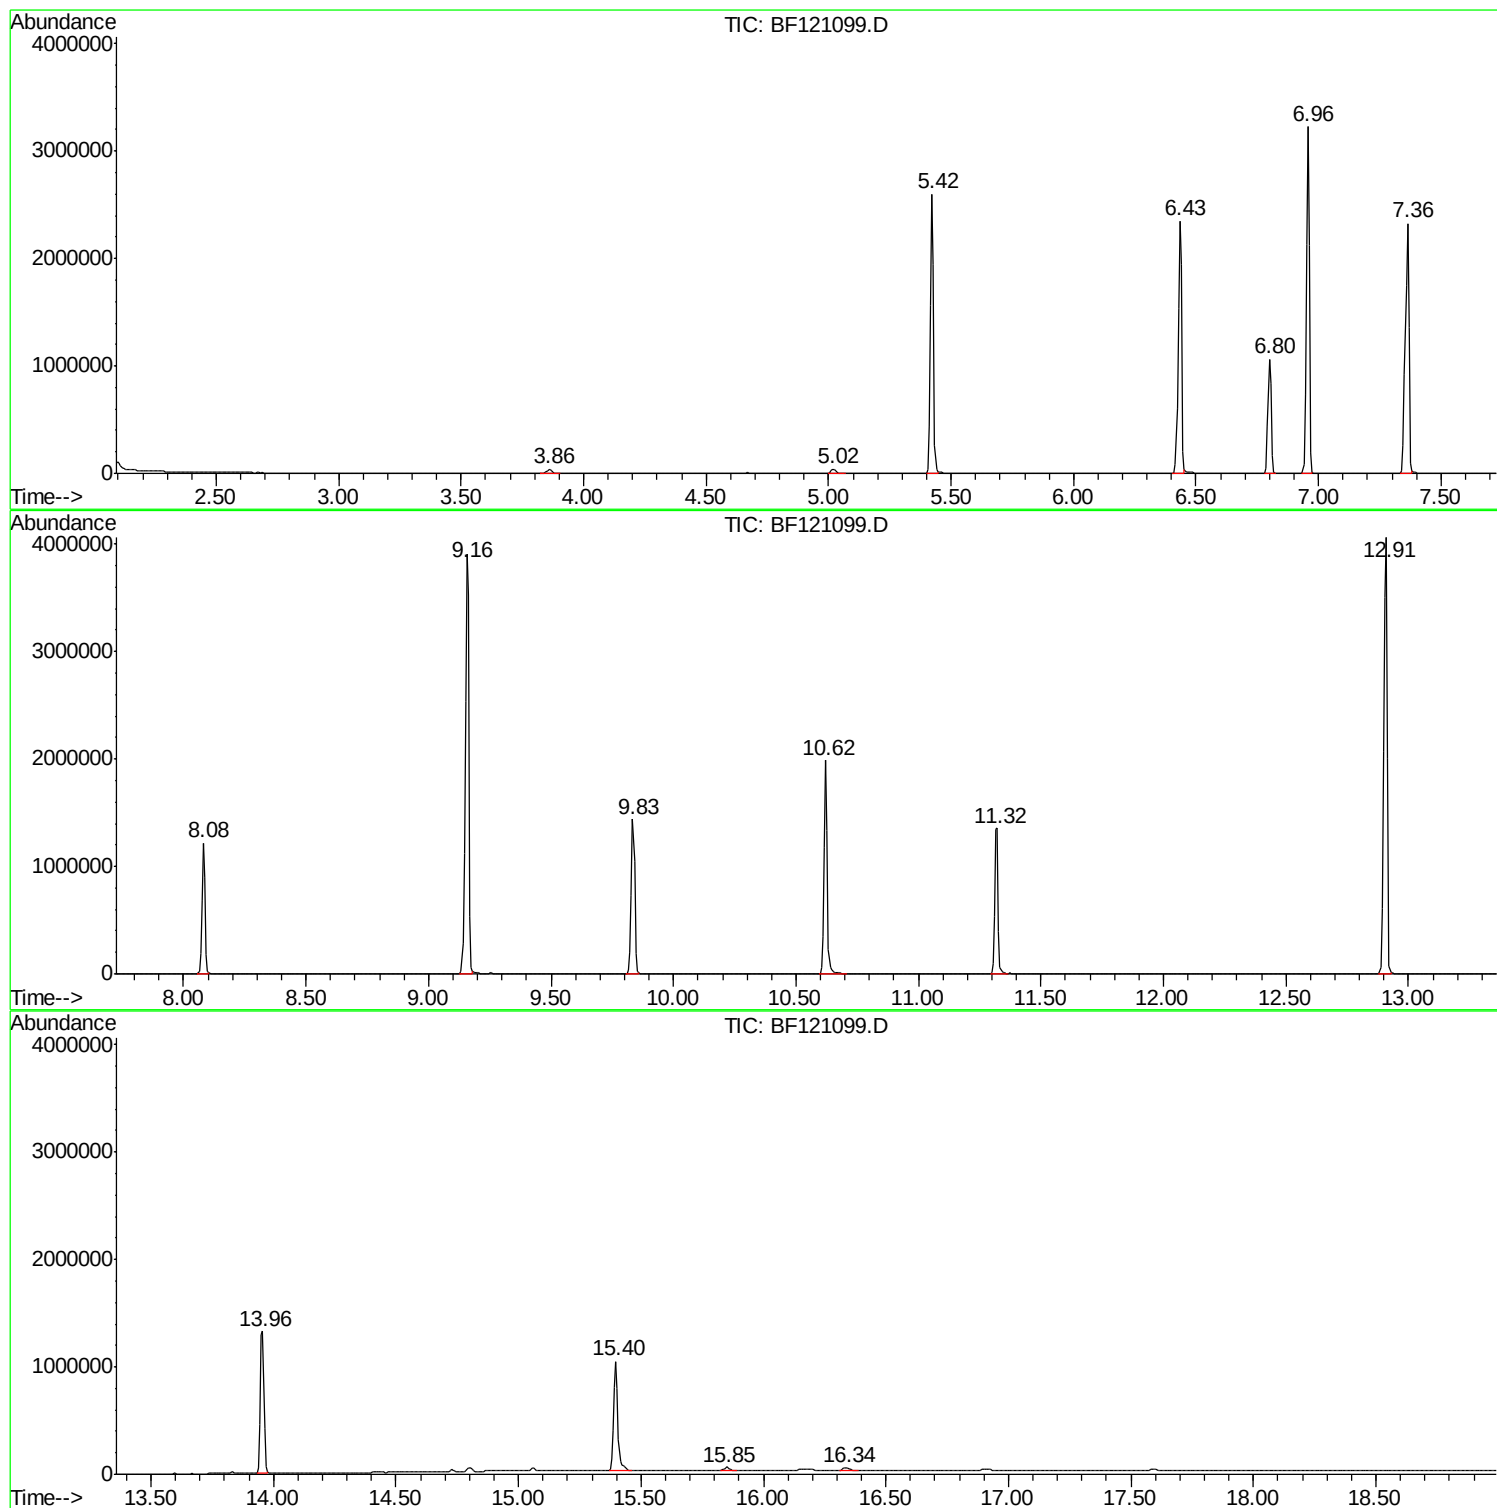

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072920\
Data File : BF121099.D
Acq On : 29 Jul 2020 13:37
Operator : JU/CG
Sample : PB130545BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130545BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072920\
Data File : BF121099.D
Acq On : 29 Jul 2020 13:37
Operator : JU/CG
Sample : PB130545BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130545BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc