


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072920\
 Data File : BF121094.D
 Acq On : 29 Jul 2020 10:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

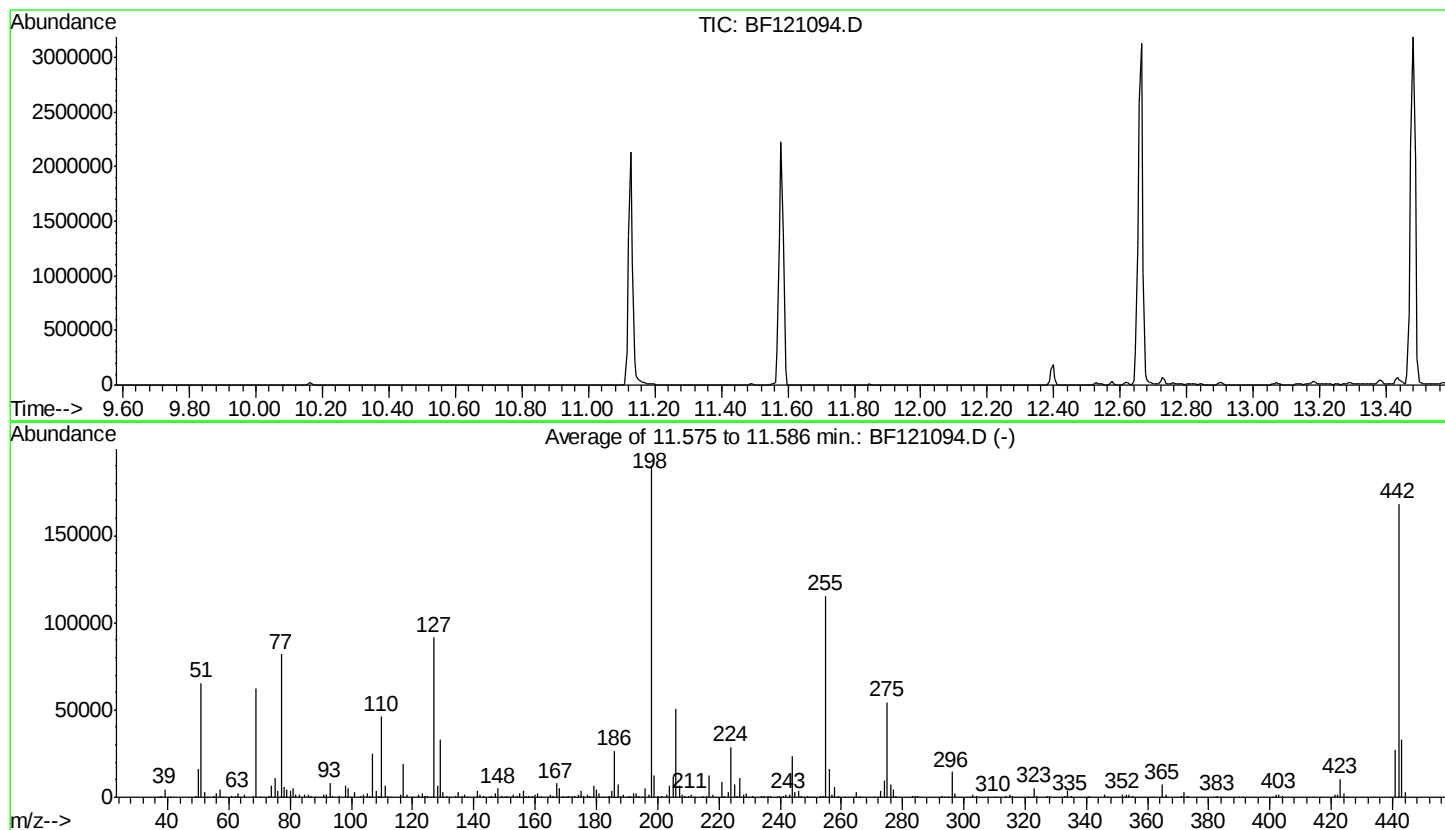

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	65576	PASS
68	69	0.00	2	1.7	1054	PASS
69	198	0.00	100	33.0	62624	PASS
70	69	0.00	2	0.5	300	PASS
127	198	10	80	48.2	91546	PASS
197	198	0.00	2	0.6	1174	PASS
198	198	100	100	100.0	189994	PASS
199	198	5	9	6.7	12700	PASS
275	198	10	60	28.7	54594	PASS
365	198	1	100	3.8	7249	PASS
441	198	0.01	100	14.2	27006	PASS
442	198	50	100	88.4	167989	PASS
443	442	15	24	19.5	32721	PASS