


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072920\
 Data File : BF121101.D
 Acq On : 29 Jul 2020 14:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

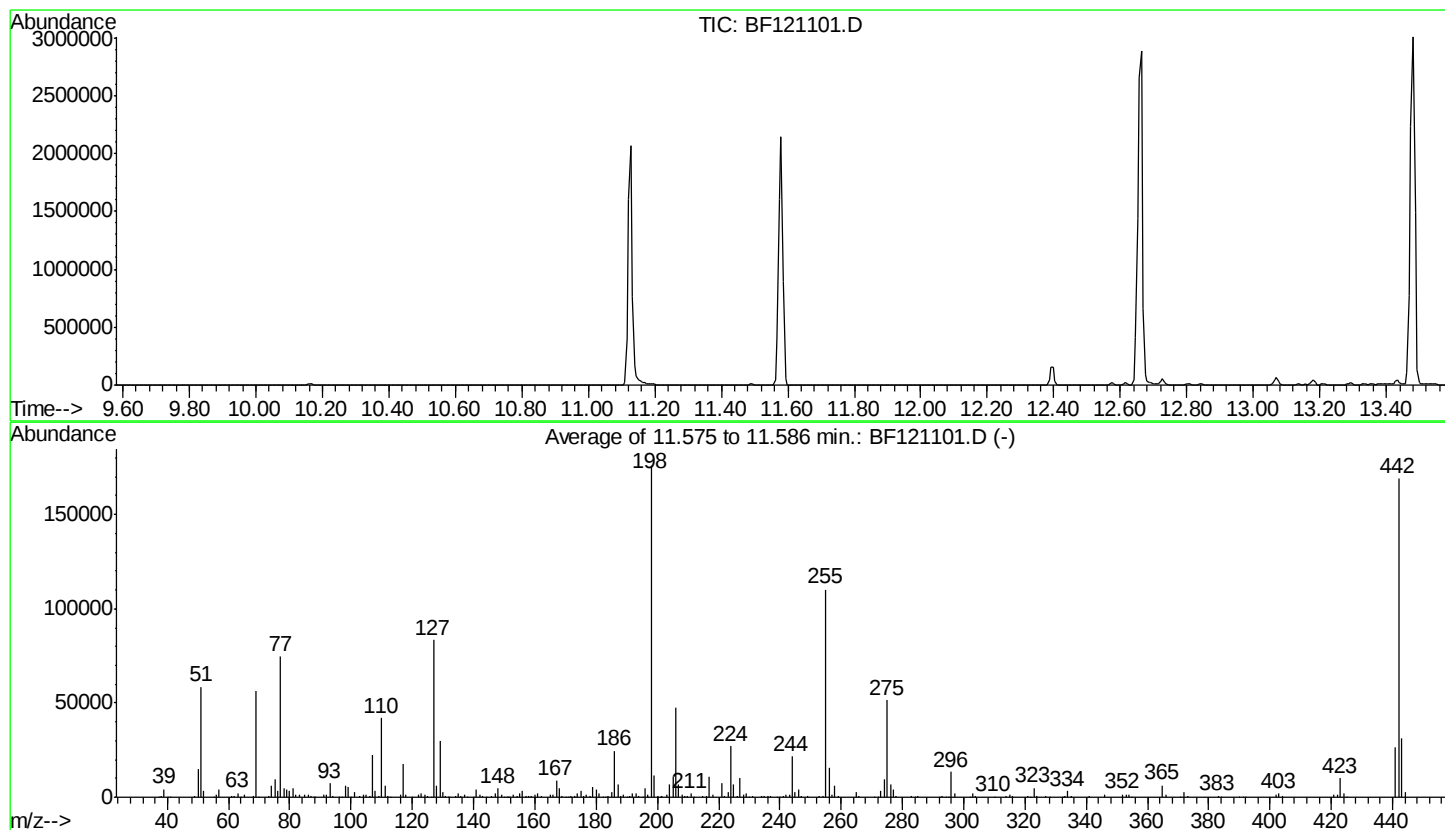

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	58626	PASS
68	69	0.00	2	1.4	775	PASS
69	198	0.00	100	31.9	56152	PASS
70	69	0.00	2	0.4	244	PASS
127	198	10	80	47.4	83474	PASS
197	198	0.00	2	0.8	1342	PASS
198	198	100	100	100.0	175944	PASS
199	198	5	9	6.7	11742	PASS
275	198	10	60	29.2	51306	PASS
365	198	1	100	3.7	6465	PASS
441	198	0.01	100	14.9	26220	PASS
442	198	50	100	96.0	168845	PASS
443	442	15	24	18.5	31314	PASS