
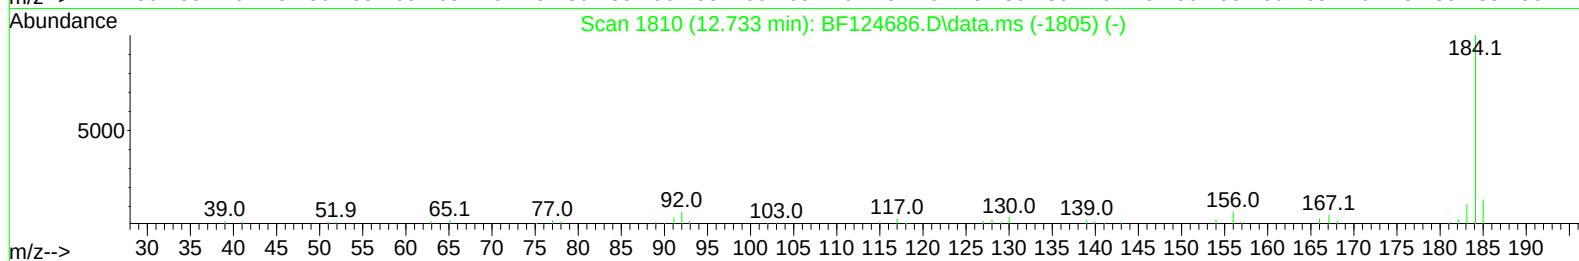
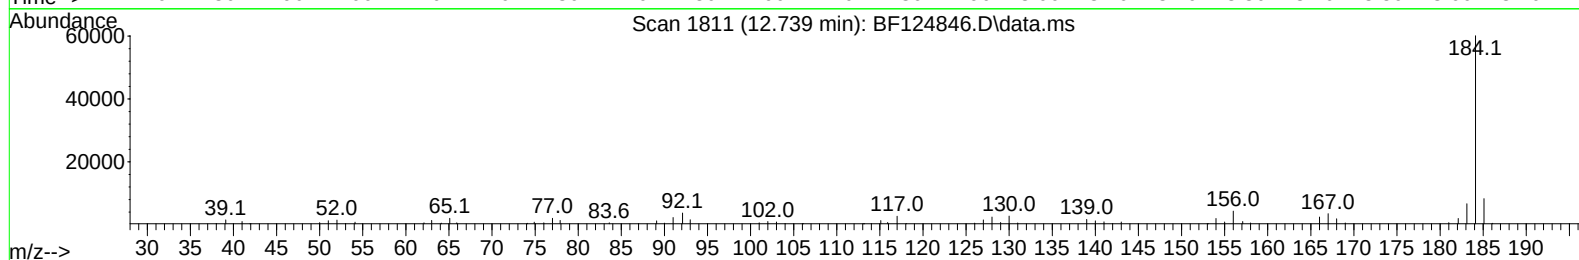


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
 Data File : BF124846.D
 Acq On : 29 Jul 2021 12:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 13:38:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 15:28:57 2021
 Response via : Initial Calibration

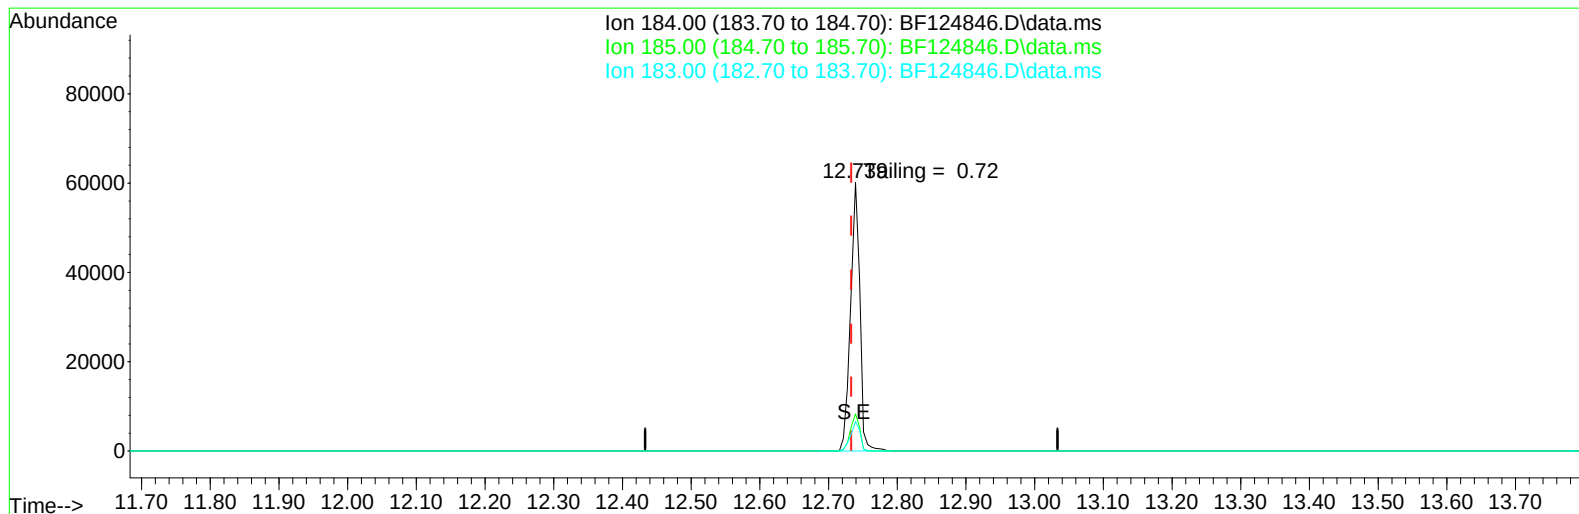

TIC: BF124846.D\data.ms

(77) Benzidine




12.739min (+ 0.006) 0.00 ng

response 56978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.84
183.00	10.10	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
Data File : BF124846.D
Acq On : 29 Jul 2021 12:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 13:38:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

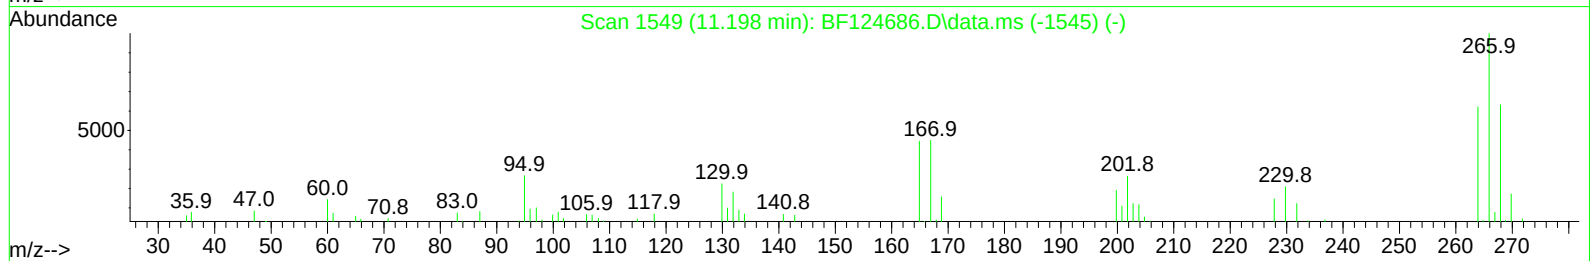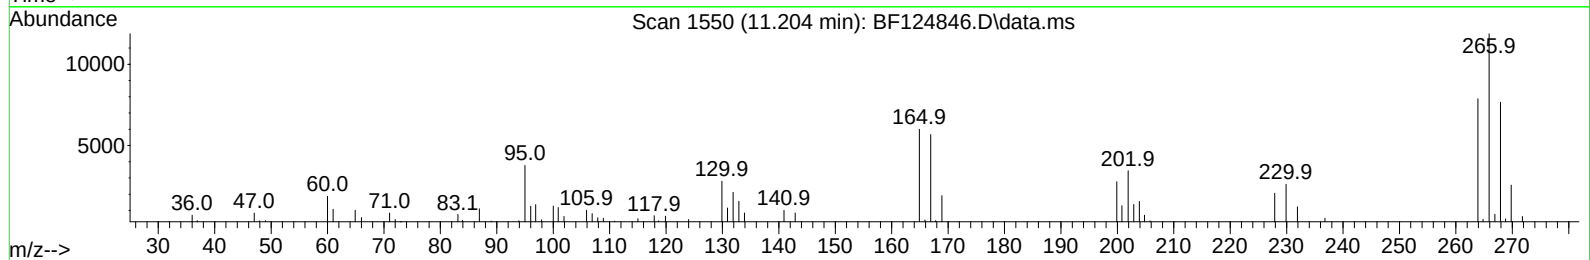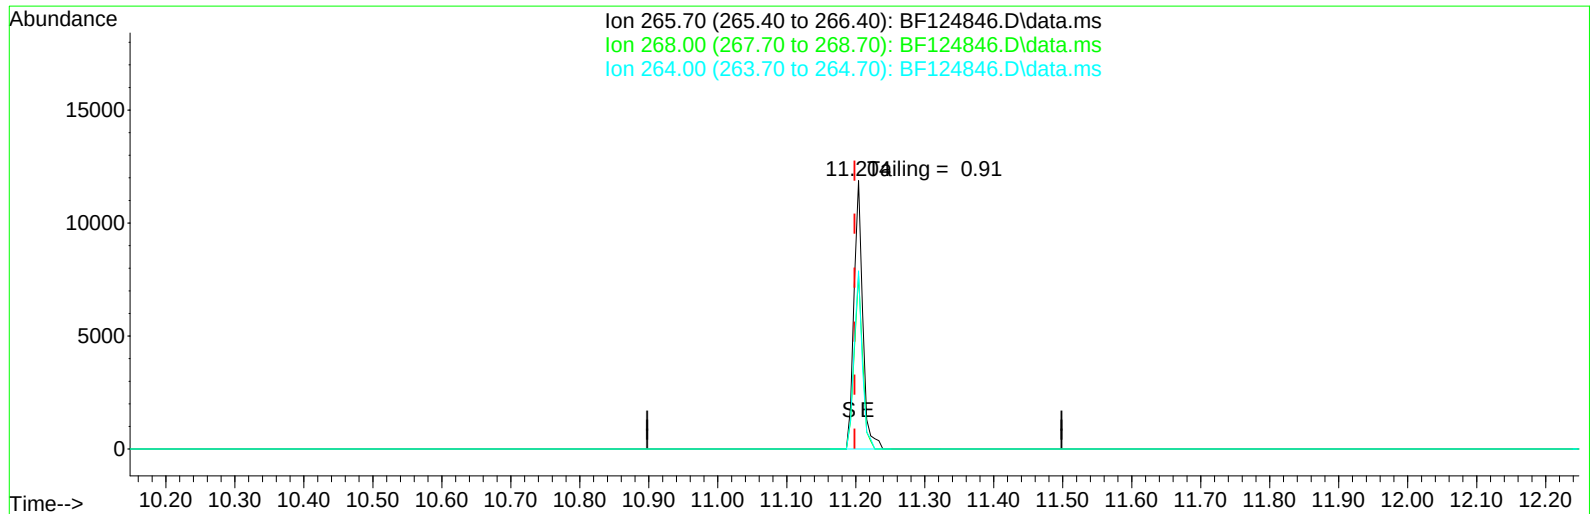

TIC: BF124846.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 0.00 ng

response 10617

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.47
264.00	69.90	66.33
0.00	0.00	0.00