

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
 Data File : BF124848.D
 Acq On : 29 Jul 2021 13:14
 Operator : JU/CG
 Sample : PB138041BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138041BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	576	582	584	rBV	212415	235176	50.77%	11.666%
2	6.504	745	751	754	rBV	205207	251206	54.23%	12.461%
3	6.869	810	813	816	rBB	51448	44669	9.64%	2.216%
4	7.439	904	910	913	rBB	155974	161222	34.80%	7.997%
5	8.157	1027	1032	1035	rBB	62884	59437	12.83%	2.948%
6	9.233	1209	1215	1218	rBV	350589	330198	71.28%	16.379%
7	9.910	1326	1330	1333	rBV	87591	71168	15.36%	3.530%
8	10.704	1460	1465	1468	rBV	225016	230201	49.70%	11.419%
9	11.398	1579	1583	1587	rBV	87920	73543	15.88%	3.648%
10	12.992	1849	1854	1857	rBV	414361	463225	100.00%	22.978%
11	14.039	2028	2032	2036	rBB	67641	55386	11.96%	2.747%
12	15.515	2279	2283	2290	rBB	31316	40547	8.75%	2.011%




Sum of corrected areas: 2015978

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
Data File : BF124848.D
Acq On : 29 Jul 2021 13:14
Operator : JU/CG
Sample : PB138041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138041BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

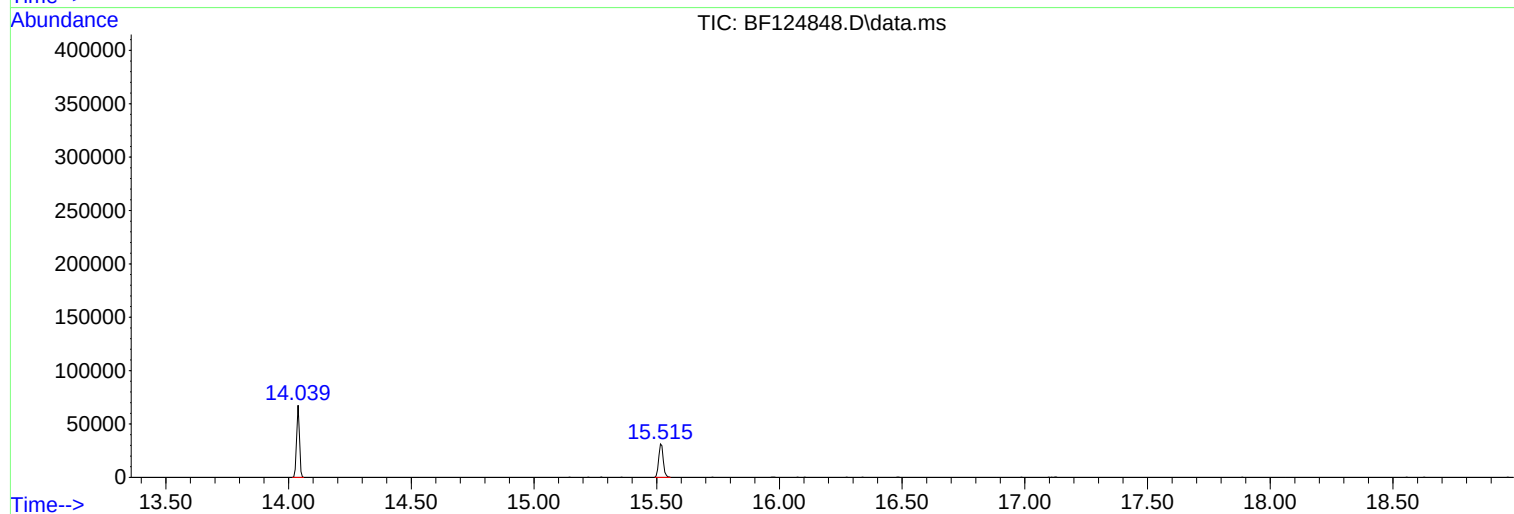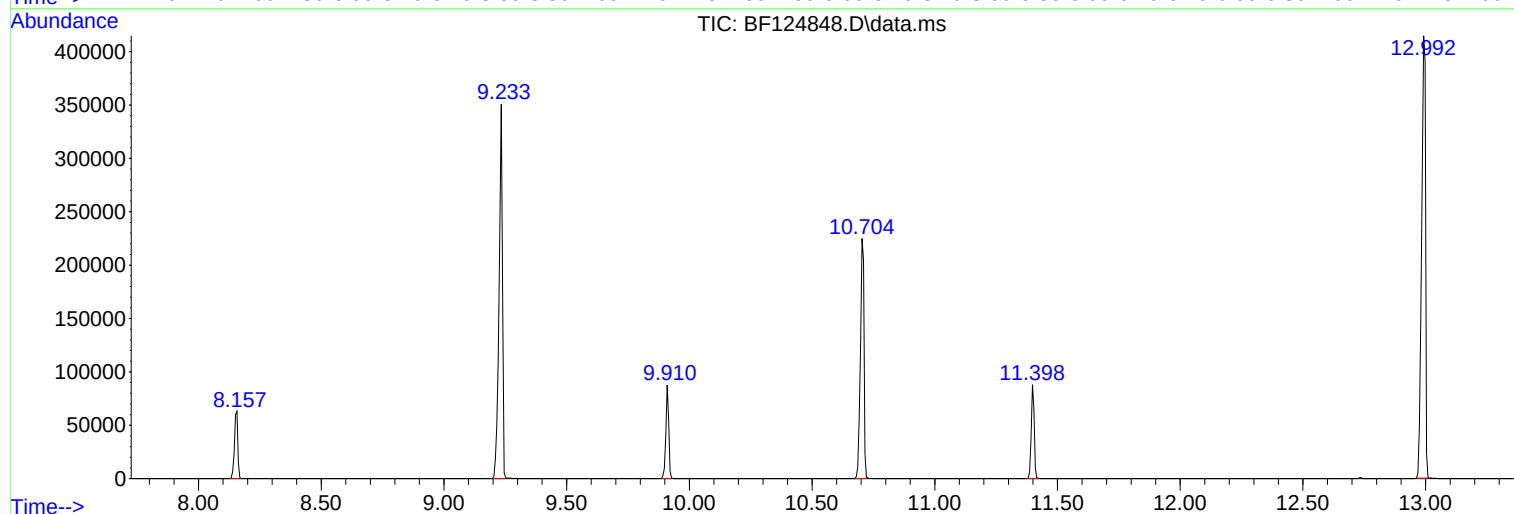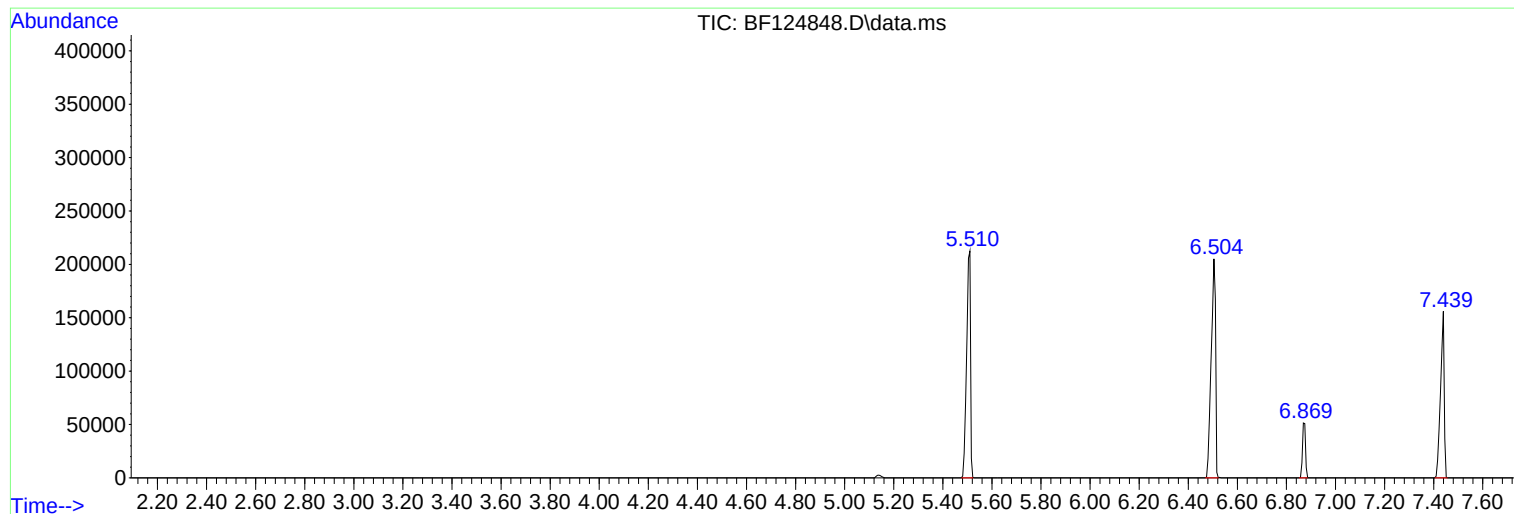

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
Data File : BF124848.D
Acq On : 29 Jul 2021 13:14
Operator : JU/CG
Sample : PB138041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138041BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
Data File : BF124848.D
Acq On : 29 Jul 2021 13:14
Operator : JU/CG
Sample : PB138041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138041BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------