
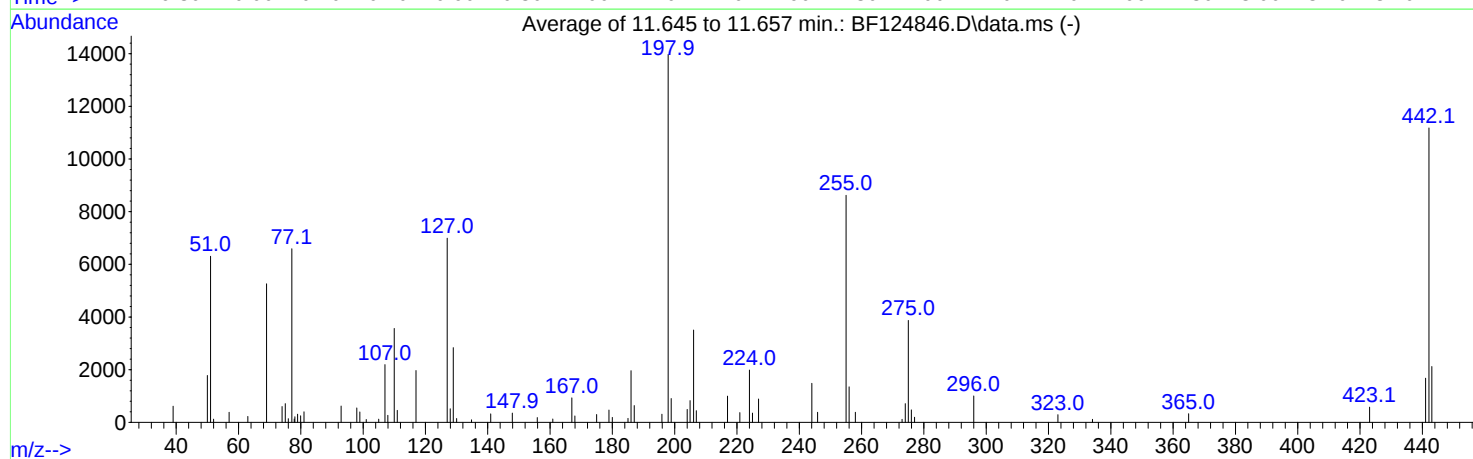


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
 Data File : BF124846.D
 Acq On : 29 Jul 2021 12:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

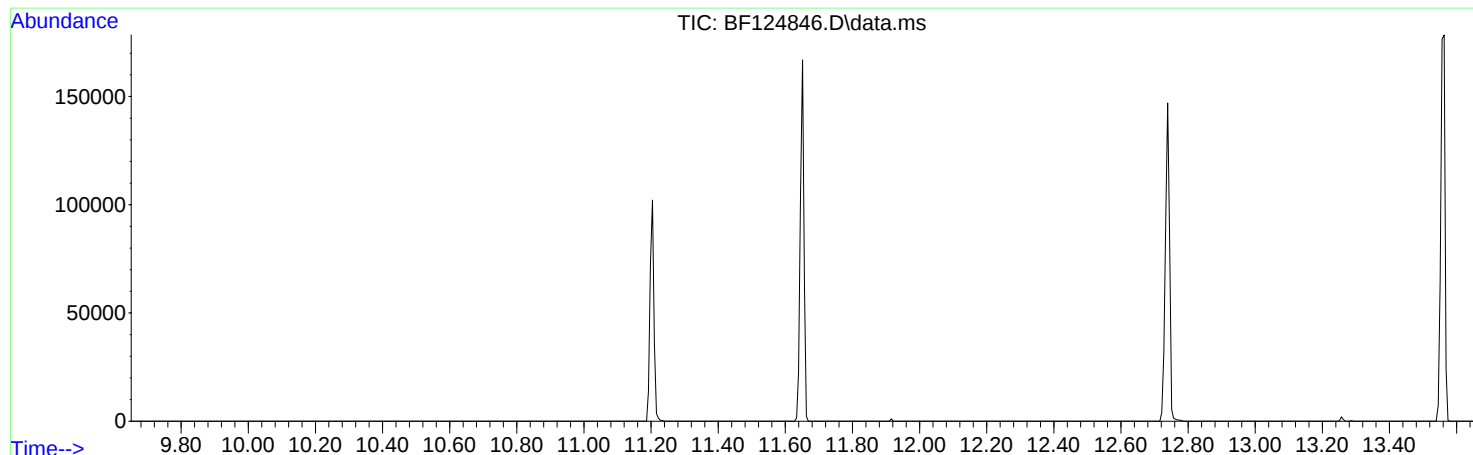




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	6306	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.7	5263	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	6995	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13968	PASS
199	198	5	9	6.5	905	PASS
275	198	10	60	27.7	3873	PASS
365	198	1	100	2.4	331	PASS
441	198	0.01	100	12.0	1675	PASS
442	442	50	100	100.0	11176	PASS
443	442	15	24	19.0	2119	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
 Data File : BF124846.D
 Acq On : 29 Jul 2021 12:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 29 13:38:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 15:28:57 2021
 Response via : Initial Calibration

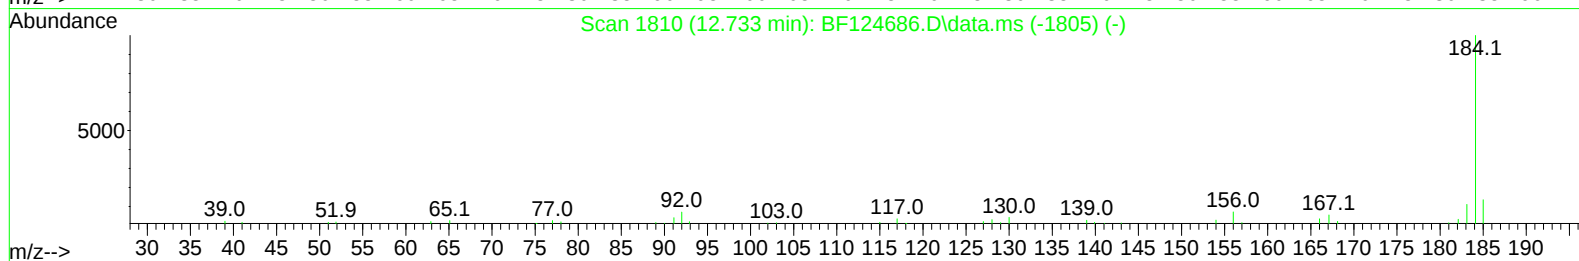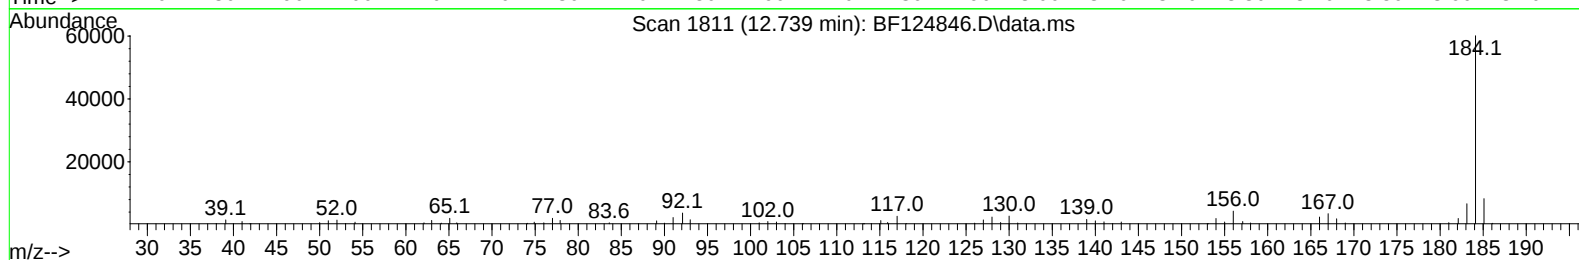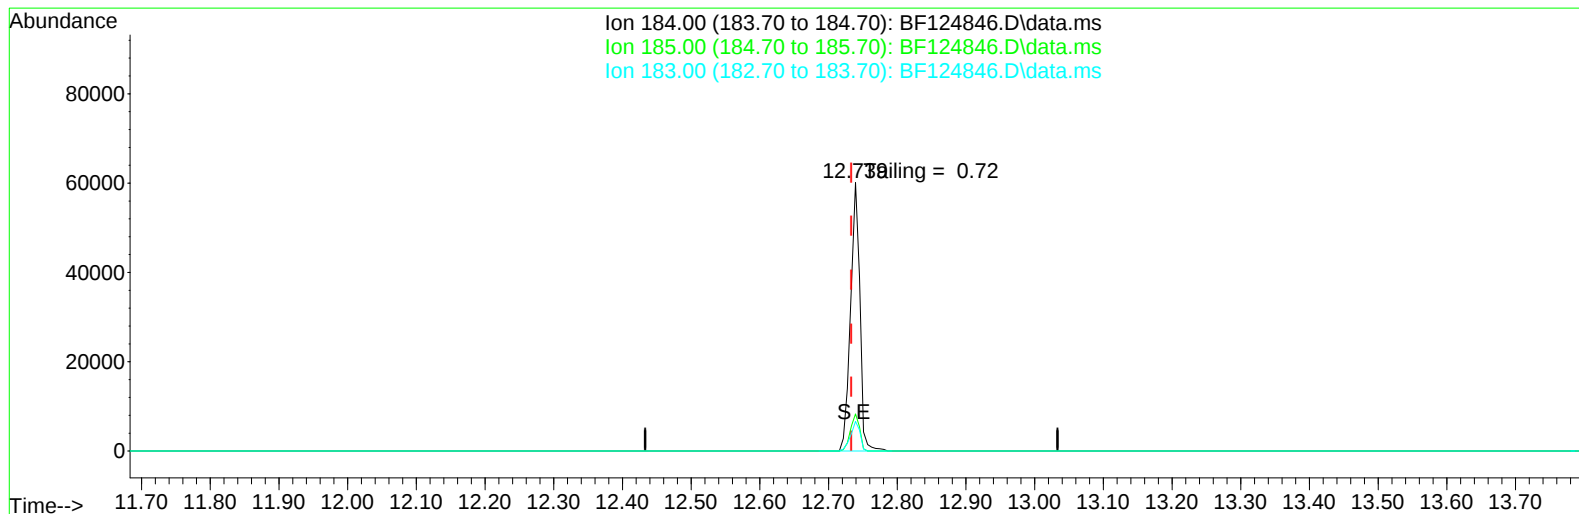

TIC: BF124846.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng




response 56978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.84
183.00	10.10	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072921\
Data File : BF124846.D
Acq On : 29 Jul 2021 12:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 13:38:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

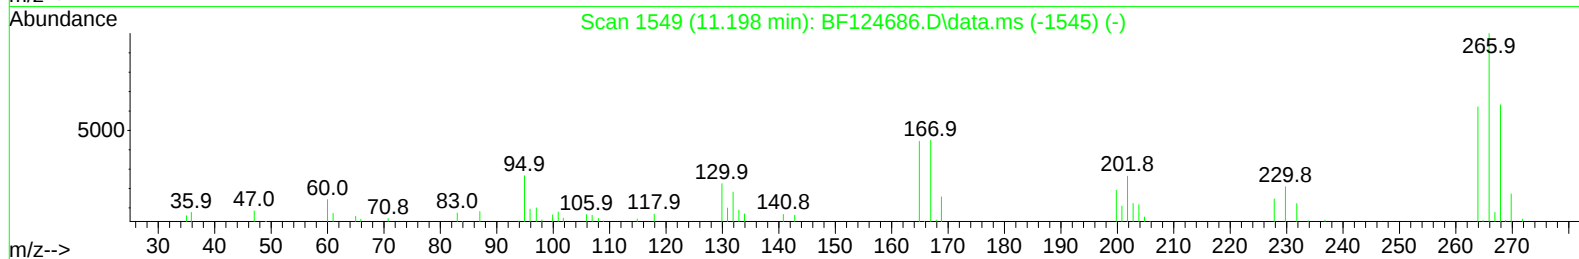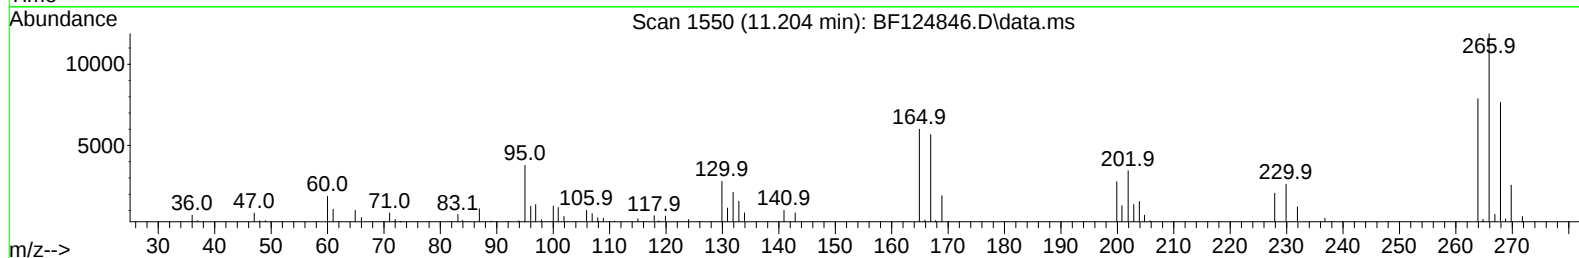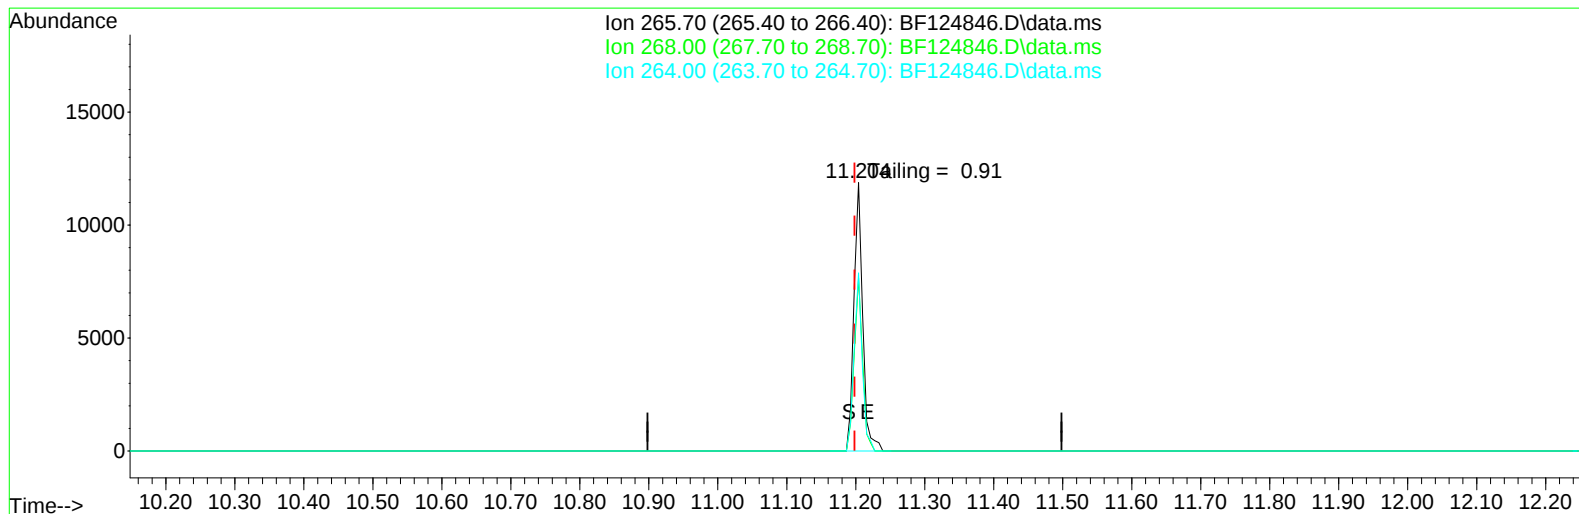

TIC: BF124846.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 0.00 ng

response 10617

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.47
264.00	69.90	66.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/29/2021	BNA_F	<u>BF124846.D</u>
Compound Name	Response	Retention Time
DDT	31925	13.56
DDD	472	13.25
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
472	32397	1.46