
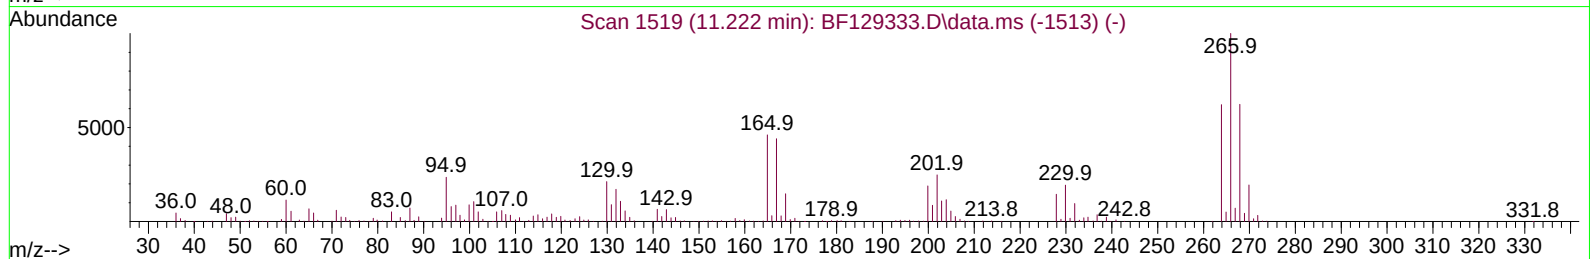
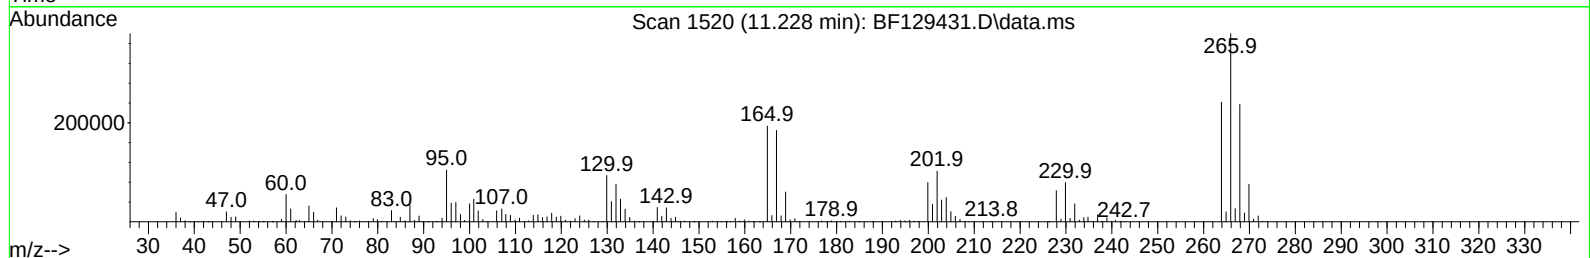


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129431.D
Acq On : 29 Jul 2022 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 18:56:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

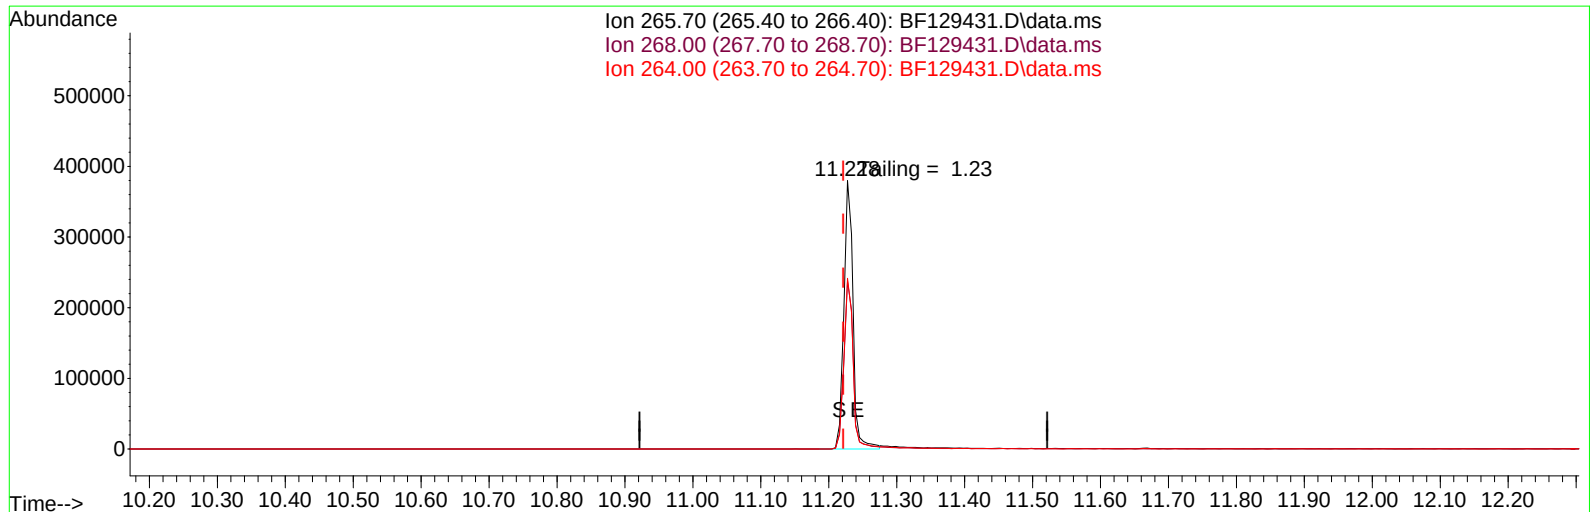

TIC: BF129431.D\data.ms

(70) Pentachlorophenol (C)




11.228min (+ 0.006) 361457.60 ng

response 361377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.53
264.00	61.80	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
 Data File : BF129431.D
 Acq On : 29 Jul 2022 09:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 18:56:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

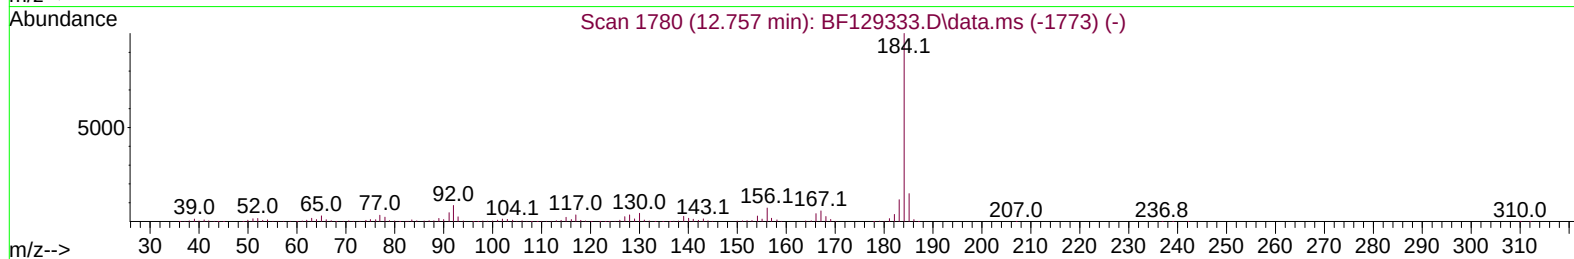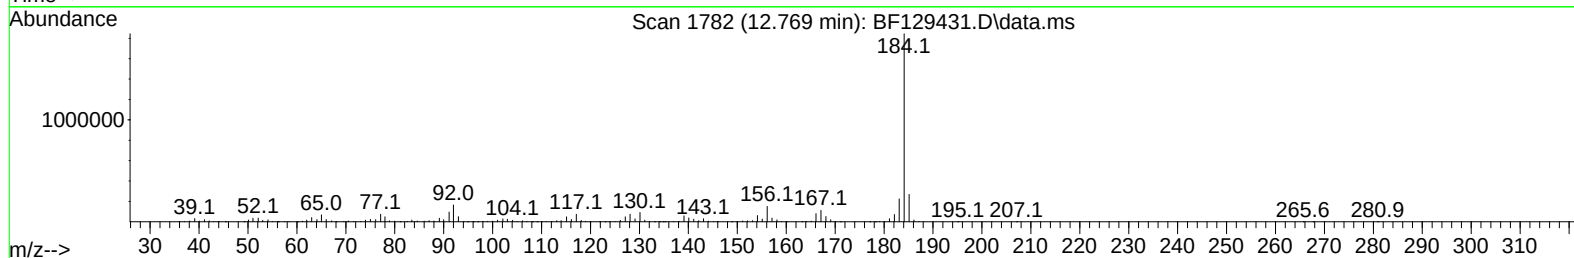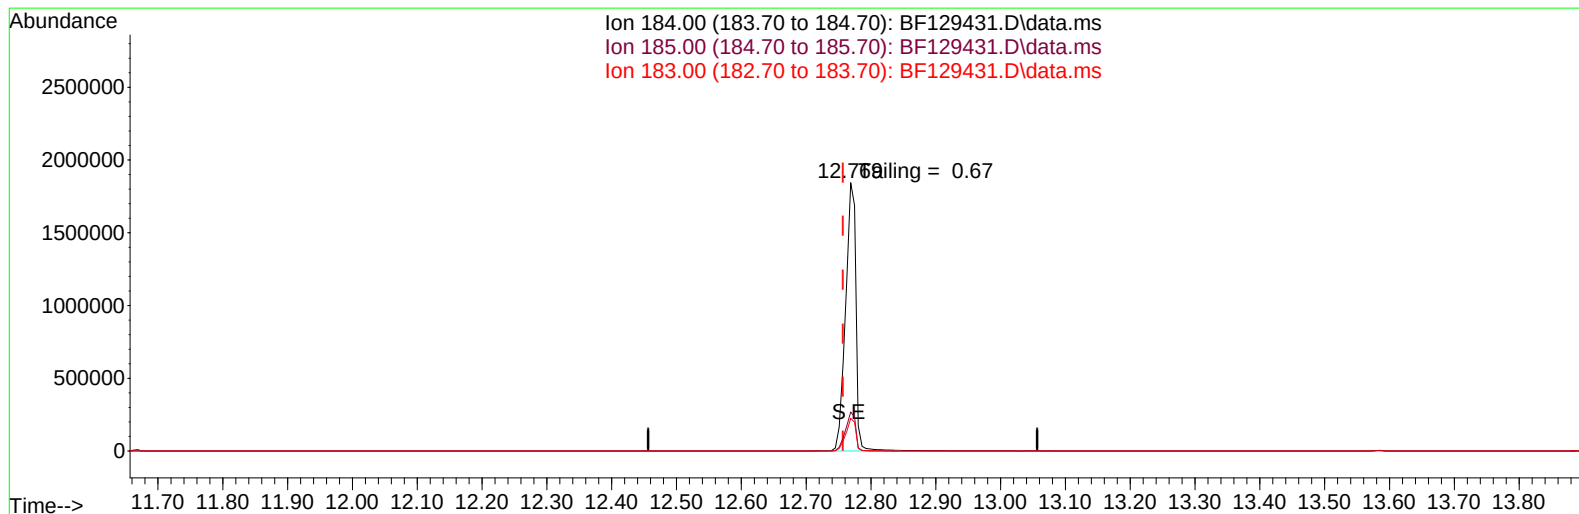

TIC: BF129431.D\data.ms

(77) Benzidine**12.769min (+ 0.012) 119473.28 ng****response 2059699**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.59
183.00	11.60	12.18
0.00	0.00	0.00