

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
 Data File : BF129433.D
 Acq On : 29 Jul 2022 10:13
 Operator : CG\JU
 Sample : PB146528BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146528BL

Quant Time: Jul 29 18:18:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	206818	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	852446	20.000	ng	0.00
39) Acenaphthene-d10	9.927	164	462478	20.000	ng	0.00
64) Phenanthrene-d10	11.421	188	801109	20.000	ng	0.00
76) Chrysene-d12	14.068	240	601473	20.000	ng	0.00
86) Perylene-d12	15.562	264	487731	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	1627337	128.177	ng	0.03
7) Phenol-d6	6.528	99	2042448	127.988	ng	0.01
23) Nitrobenzene-d5	7.451	82	1367898	87.597	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	564038	126.853	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	2358618	78.894	ng	0.00
79) Terphenyl-d14	13.010	244	2622372	82.253	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129433.D
Acq On : 29 Jul 2022 10:13
Operator : CG\JU
Sample : PB146528BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146528BL

Quant Time: Jul 29 18:18:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration




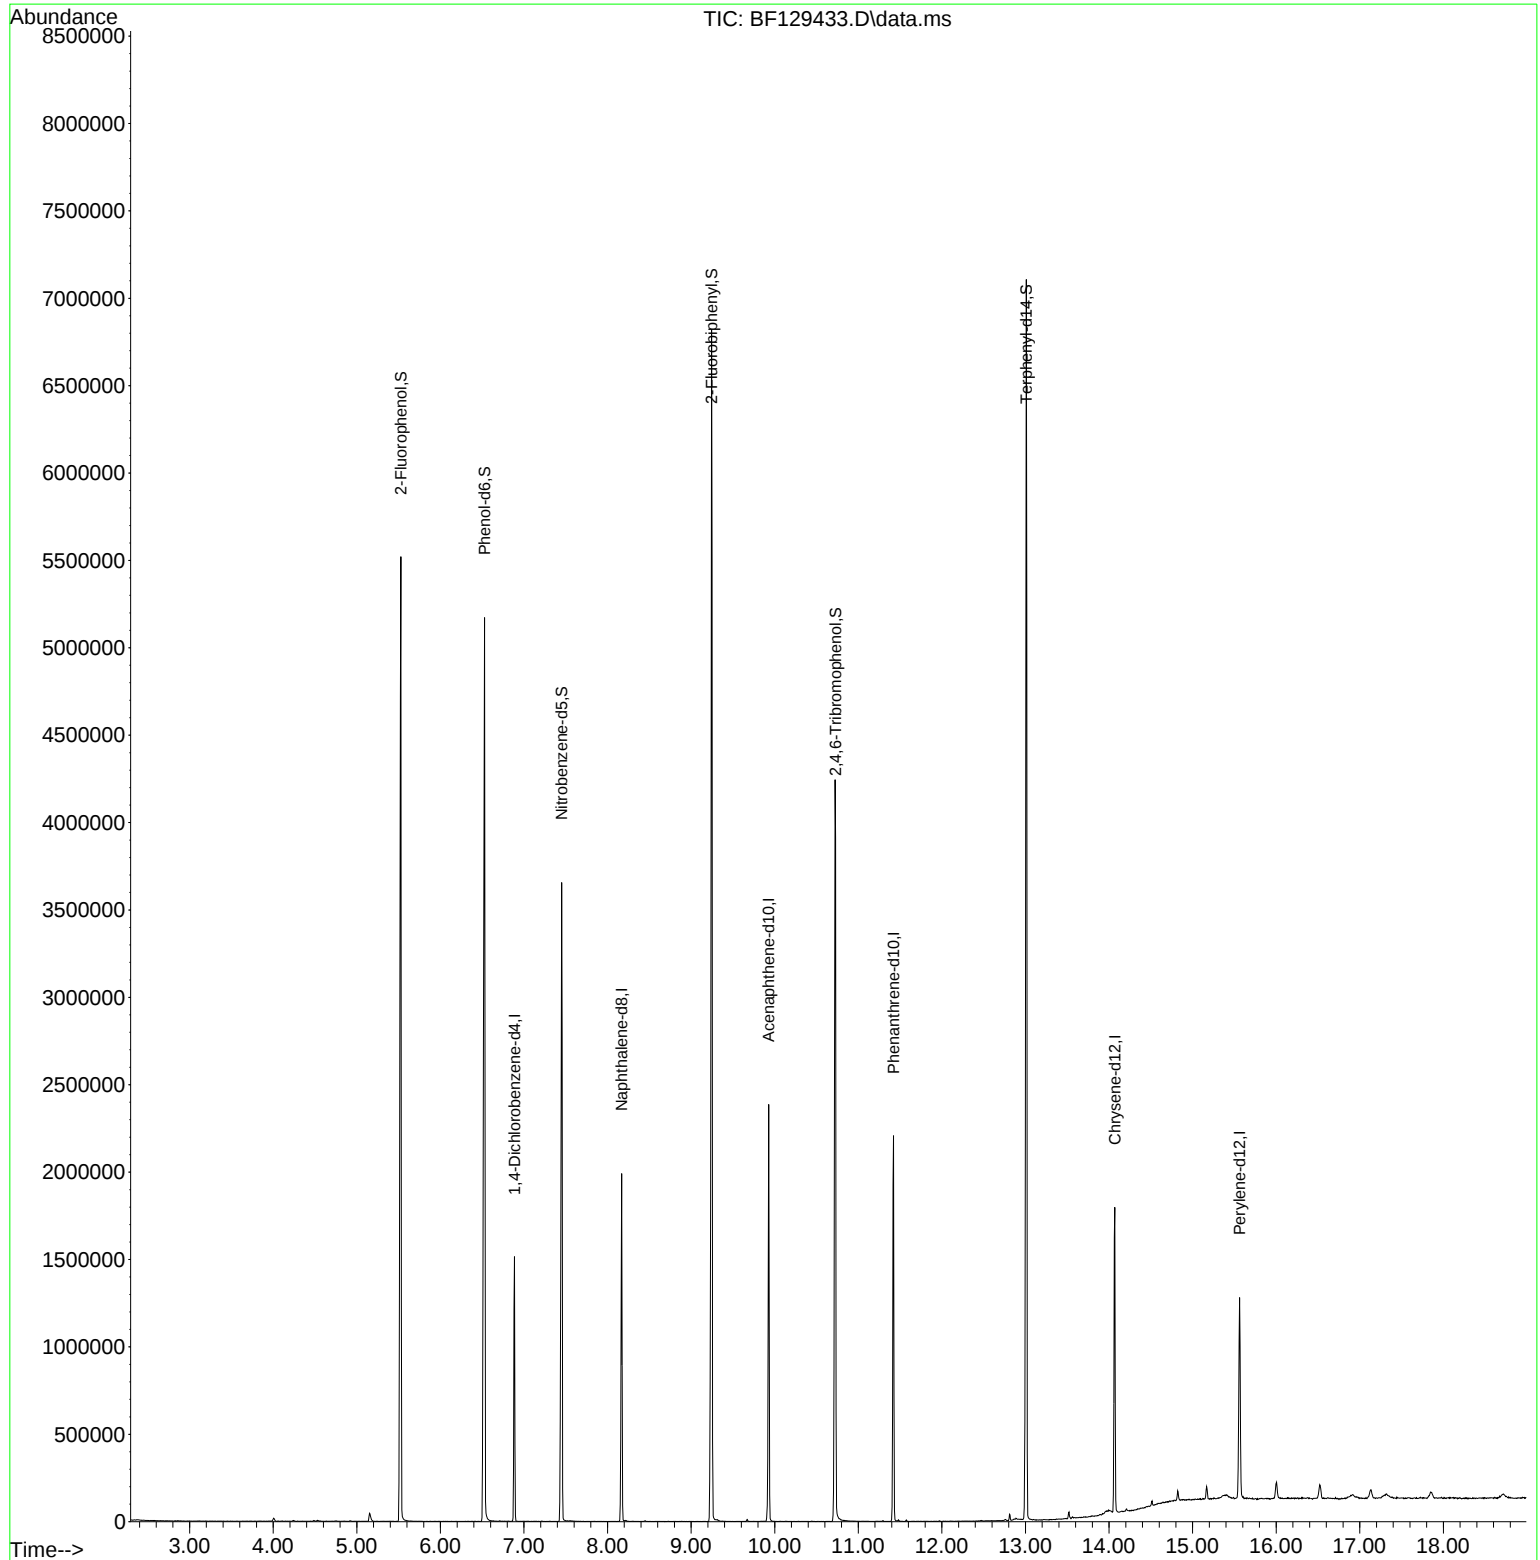


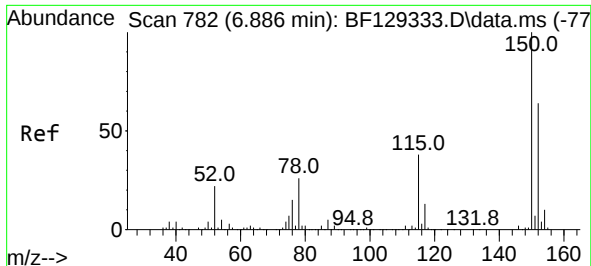

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.886 min Scan# 782
 Delta R.T. 0.000 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13




Instrument :
 BNA_F
 ClientSampleId :
 PB146528BL

Tgt Ion:152 Resp: 206818
 Ion Ratio Lower Upper
 152 100
 150 155.0 123.7 185.5
 115 61.5 49.9 74.9

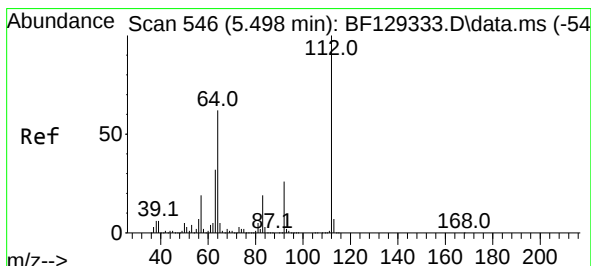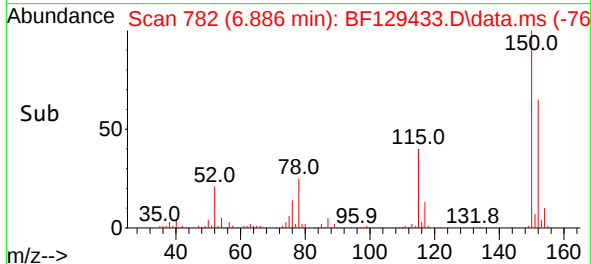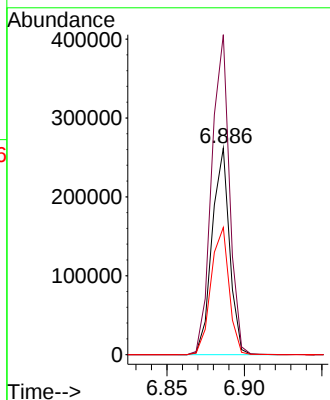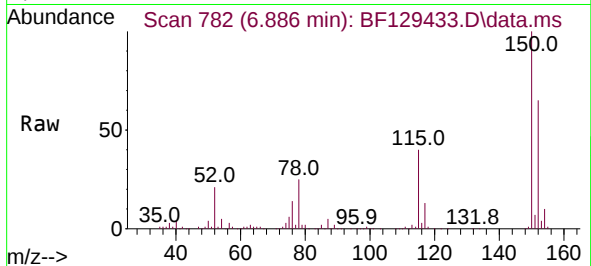

#5
 2-Fluorophenol
 Concen: 128.177 ng
 RT: 5.528 min Scan# 551
 Delta R.T. 0.029 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13

Tgt Ion:112 Resp: 1627337
 Ion Ratio Lower Upper
 112 100
 64 60.0 53.3 79.9
 63 31.5 28.0 42.0


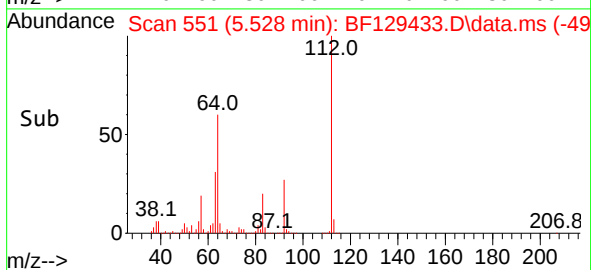
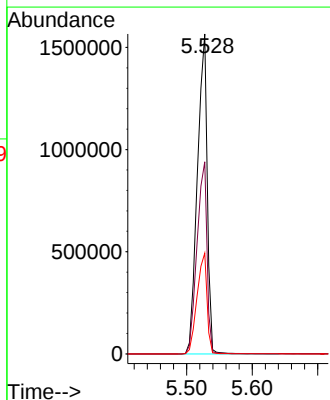
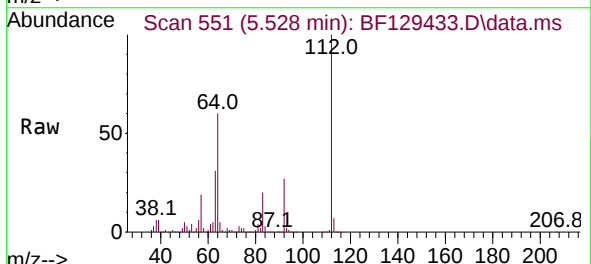




#7
Phenol-d6
Concen: 127.988 ng
RT: 6.528 min Scan# 719
Delta R.T. 0.012 min
Lab File: BF129433.D
Acq: 29 Jul 2022 10:13




Instrument :
BNA_F
ClientSampleId :
PB146528BL

Tgt Ion: 99 Resp: 2042448
Ion Ratio Lower Upper
99 100
42 19.5 17.3 25.9
71 36.5 28.9 43.3

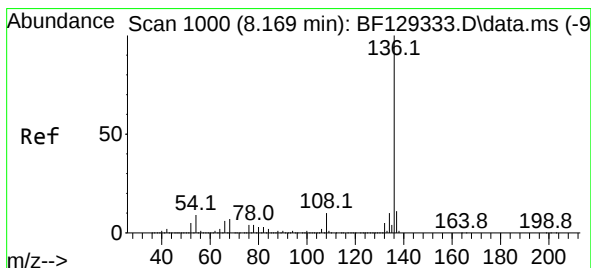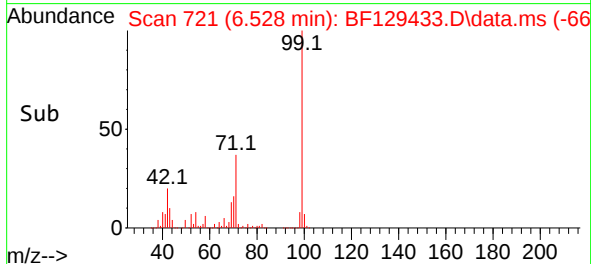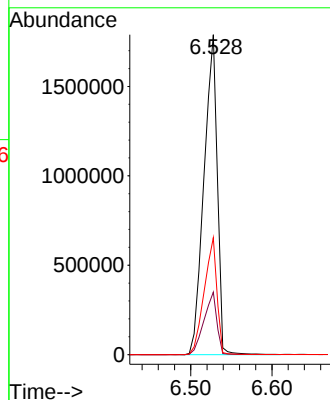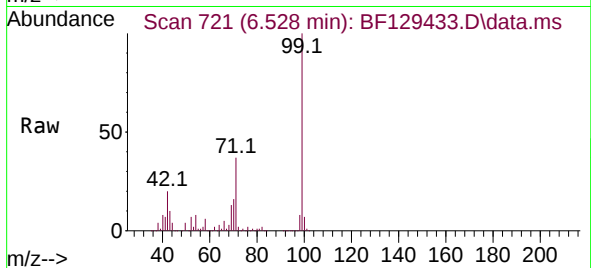

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1000
Delta R.T. -0.000 min
Lab File: BF129433.D
Acq: 29 Jul 2022 10:13

Tgt Ion:136 Resp: 852446
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 8.2 7.5 11.3
68 5.7 4.7 7.1

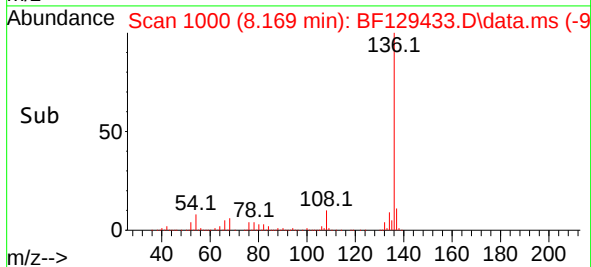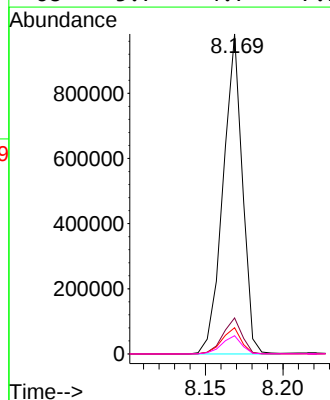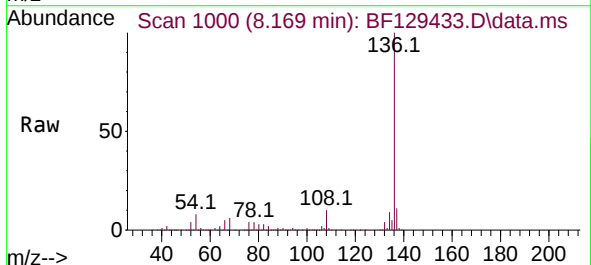







#23
 Nitrobenzene-d5
 Concen: 87.597 ng
 RT: 7.451 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13

Instrument :
 BNA_F
 ClientSampleId :
 PB146528BL

Tgt Ion: 82 Resp: 1367898




Ion	Ratio	Lower	Upper
82	100		
128	44.2	34.0	51.0
54	52.5	46.9	70.3

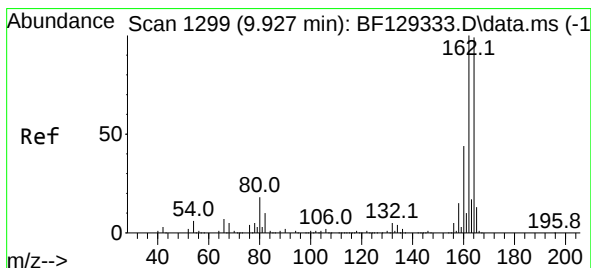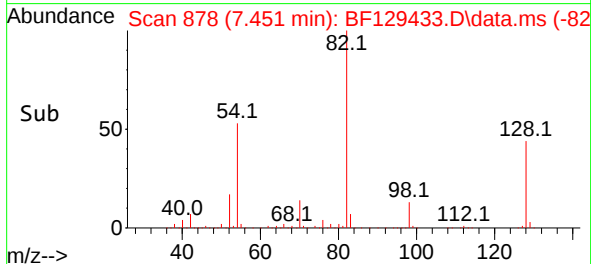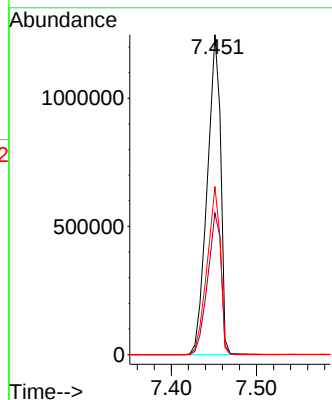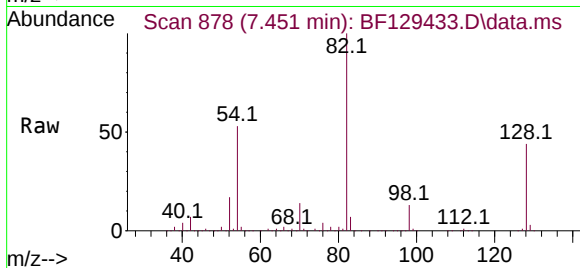


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.927 min Scan# 1299
 Delta R.T. -0.000 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13

Tgt Ion: 164 Resp: 462478

Ion	Ratio	Lower	Upper
164	100		
162	100.1	79.5	119.3
160	44.4	34.2	51.4

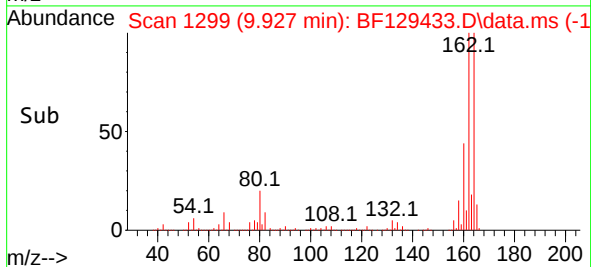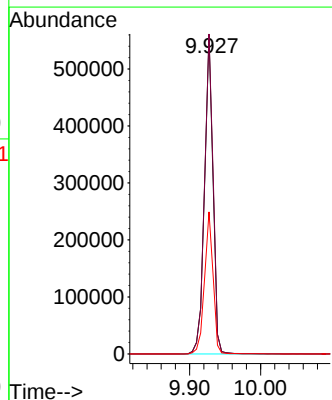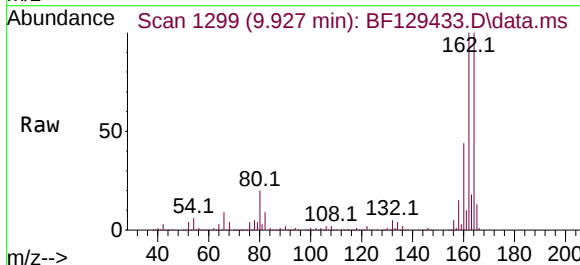

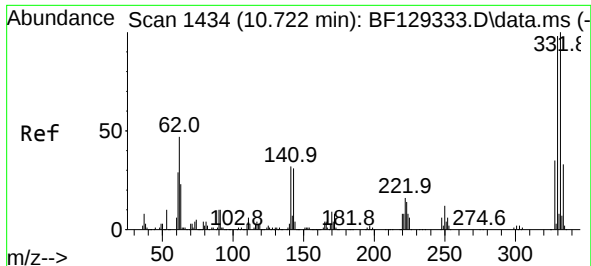

#42

2,4,6-Tribromophenol

Concen: 126.853 ng

RT: 10.727 min Scan# 1434

Delta R.T. 0.006 min

Lab File: BF129433.D

Acq: 29 Jul 2022 10:13

Instrument :

BNA_F

ClientSampleId :

PB146528BL





Tgt Ion:330 Resp: 564038

Ion Ratio Lower Upper

330 100

332 103.2 76.8 115.2

141 34.8 28.0 42.0

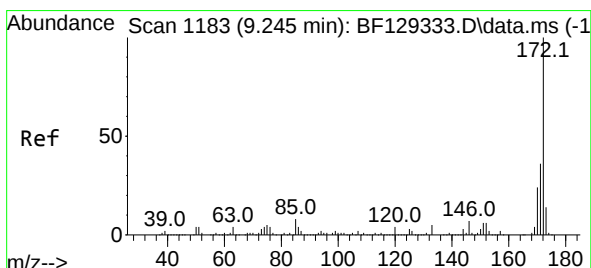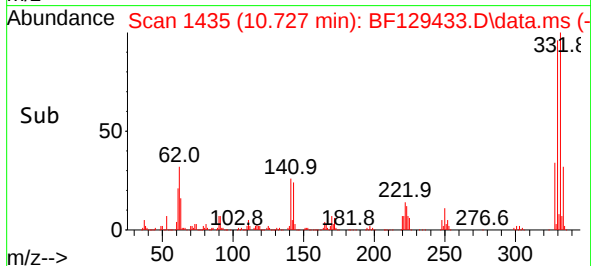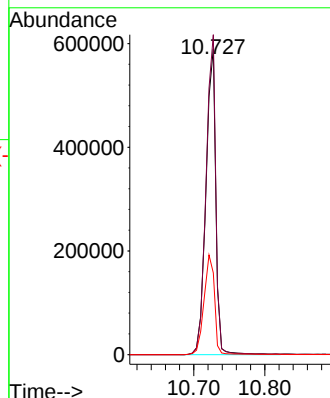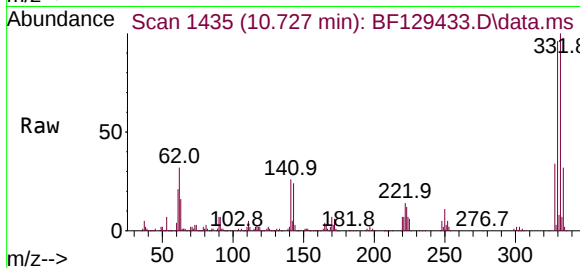

#45

2-Fluorobiphenyl

Concen: 78.894 ng

RT: 9.245 min Scan# 1183

Delta R.T. -0.000 min

Lab File: BF129433.D

Acq: 29 Jul 2022 10:13




Tgt Ion:172 Resp: 2358618


Ion Ratio Lower Upper

172 100

171 35.9 28.8 43.2

170 24.3 19.8 29.8


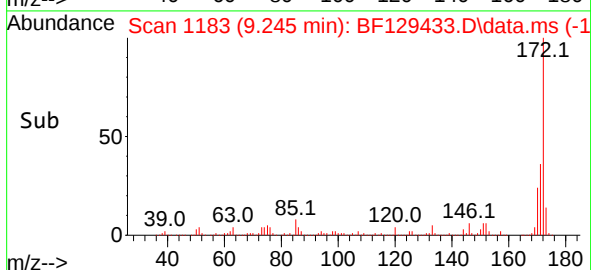
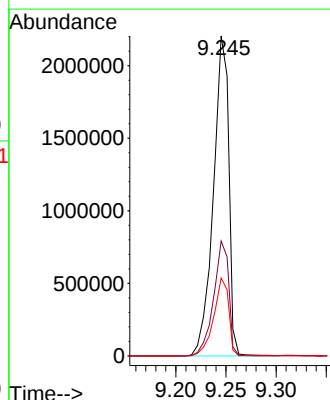
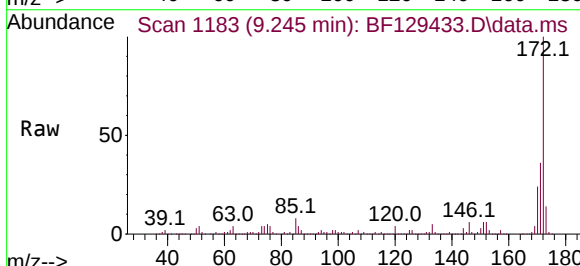


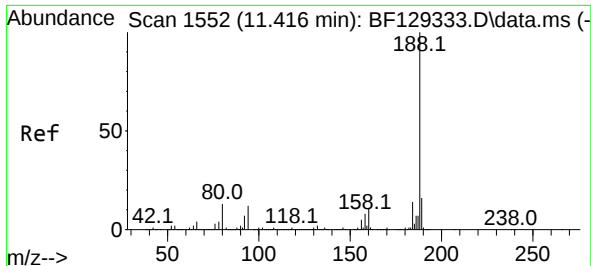

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.421 min Scan# 11
Delta R.T. 0.006 min
Lab File: BF129433.D
Acq: 29 Jul 2022 10:13




Instrument :
BNA_F
ClientSampleId :
PB146528BL


Tgt Ion:188 Resp: 801109
Ion Ratio Lower Upper
188 100
94 9.4 7.0 10.6
80 10.1 7.6 11.4

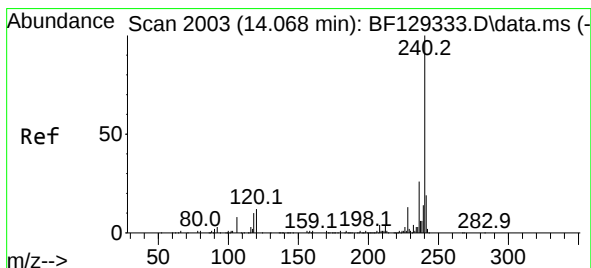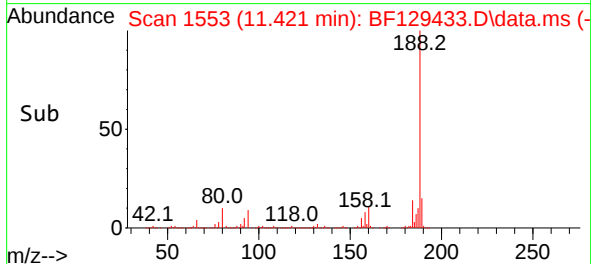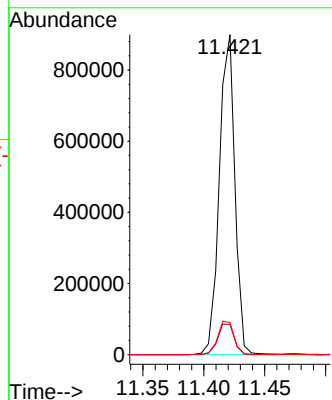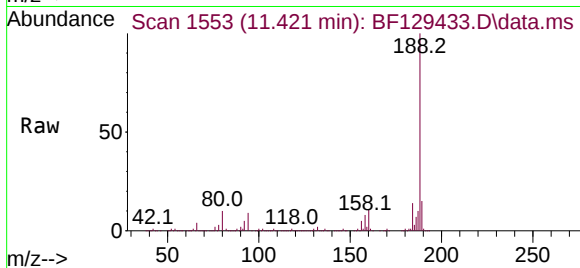

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.068 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BF129433.D
Acq: 29 Jul 2022 10:13

Tgt Ion:240 Resp: 601473
Ion Ratio Lower Upper
240 100
120 11.2 8.9 13.3
236 25.8 20.8 31.2


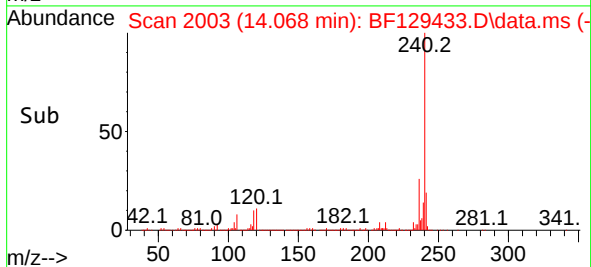
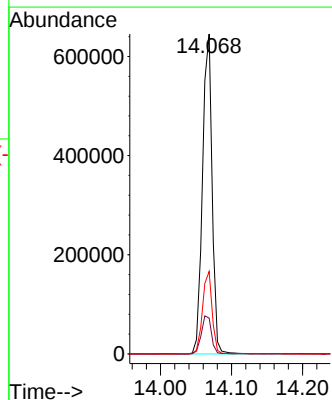
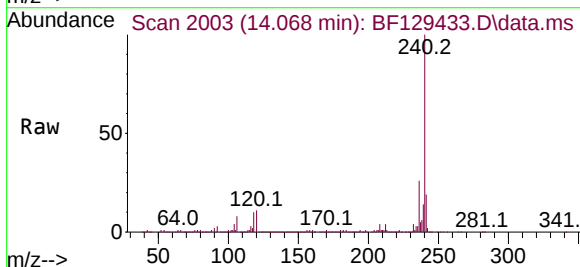


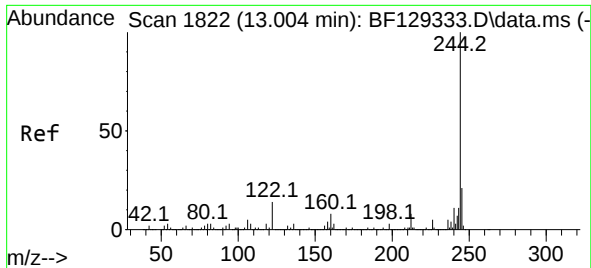

#79
 Terphenyl-d14
 Concen: 82.253 ng
 RT: 13.010 min Scan# 1822
 Delta R.T. 0.006 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13

Instrument :
 BNA_F
 ClientSampleId :
 PB146528BL

Tgt Ion:244 Resp: 2622372
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.1 9.1
 122 13.1 8.8 13.2

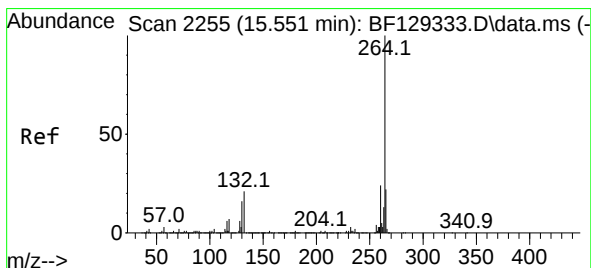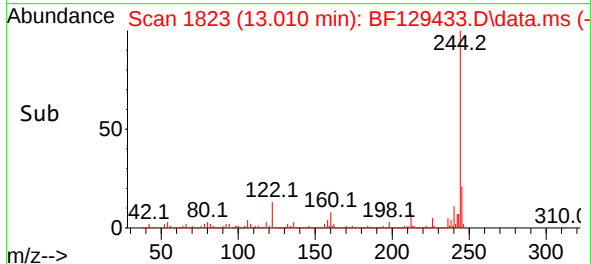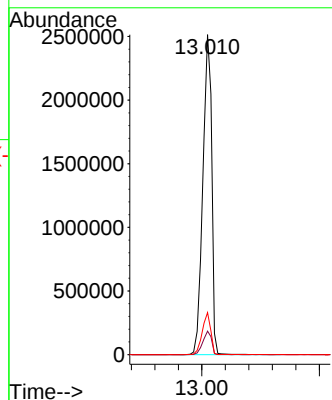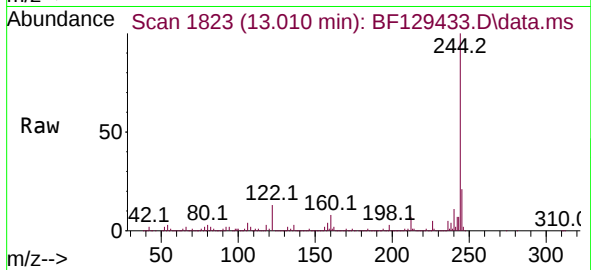

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.562 min Scan# 2257
 Delta R.T. 0.012 min
 Lab File: BF129433.D
 Acq: 29 Jul 2022 10:13

Tgt Ion:264 Resp: 487731
 Ion Ratio Lower Upper
 264 100
 260 23.8 18.4 27.6
 265 21.4 17.2 25.8

