

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
 Data File : BF129433.D
 Acq On : 29 Jul 2022 10:13
 Operator : CG\JU
 Sample : PB146528BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146528BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	545	551	554	rBV	5519997	5737947	79.93%	12.891%
2	6.528	715	721	724	rBV	5170891	5766672	80.33%	12.956%
3	6.886	778	782	785	rBV	1514777	1243270	17.32%	2.793%
4	7.451	872	878	881	rBV	3655763	3984148	55.50%	8.951%
5	8.169	995	1000	1003	rBV	1990683	1724538	24.02%	3.874%
6	9.245	1177	1183	1186	rBV	6819152	7030542	97.94%	15.795%
7	9.927	1293	1299	1302	rBV	2385583	1986309	27.67%	4.462%
8	10.721	1427	1434	1438	rBV	4244652	4406115	61.38%	9.899%
9	11.421	1546	1553	1556	rBV	2206883	1992001	27.75%	4.475%
10	13.010	1818	1823	1826	rBV	7085853	7178350	100.00%	16.127%
11	14.068	1998	2003	2006	rBV	1745580	1664085	23.18%	3.739%
12	15.168	2187	2190	2194	rVB	69412	78104	1.09%	0.175%
13	15.562	2252	2257	2266	rVB	1150116	1458933	20.32%	3.278%
14	16.004	2328	2332	2340	rVB	93571	135988	1.89%	0.306%
15	16.521	2417	2420	2426	rVB2	78900	124234	1.73%	0.279%




Sum of corrected areas: 44511236

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129433.D
Acq On : 29 Jul 2022 10:13
Operator : CG\JU
Sample : PB146528BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146528BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

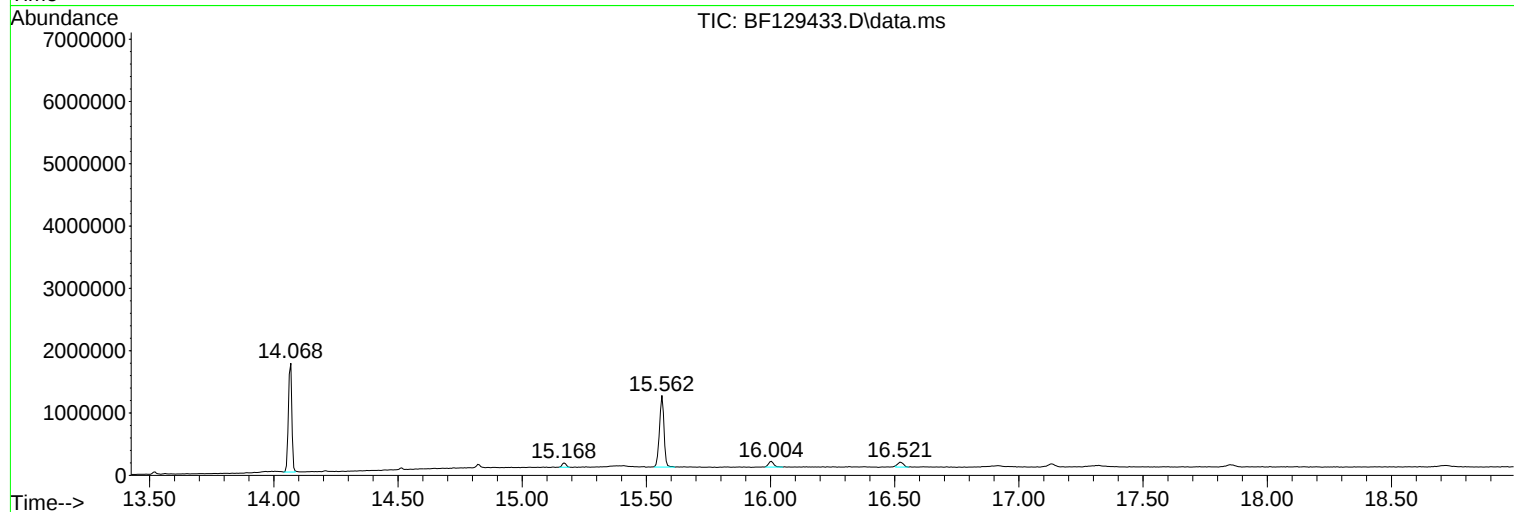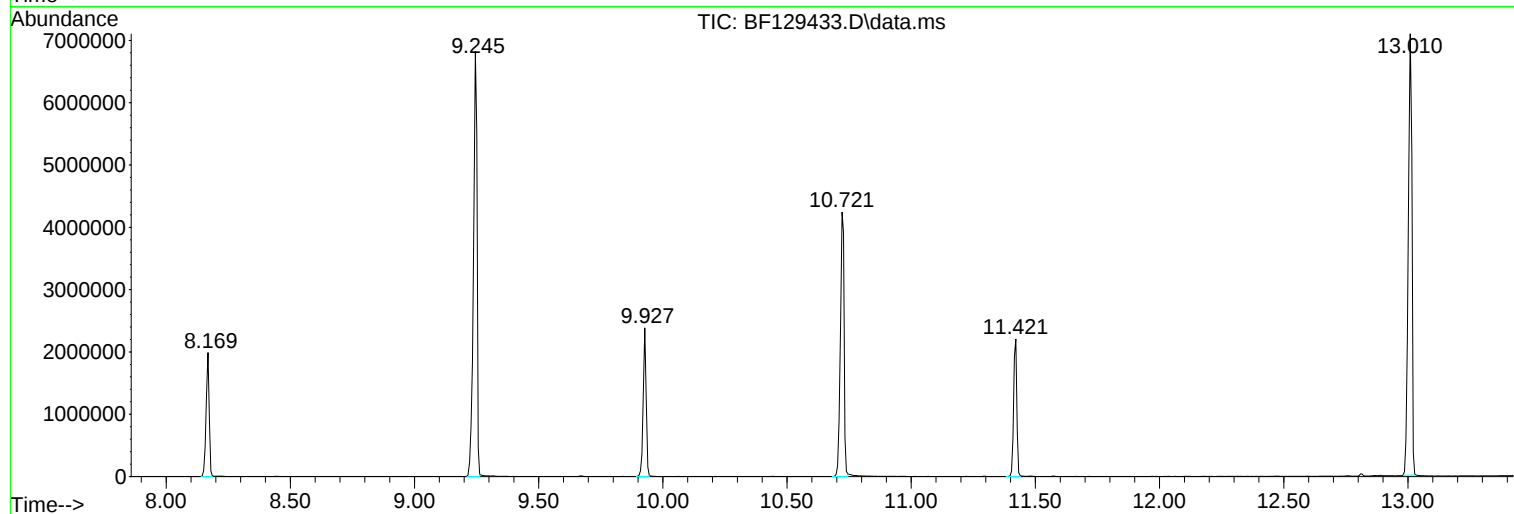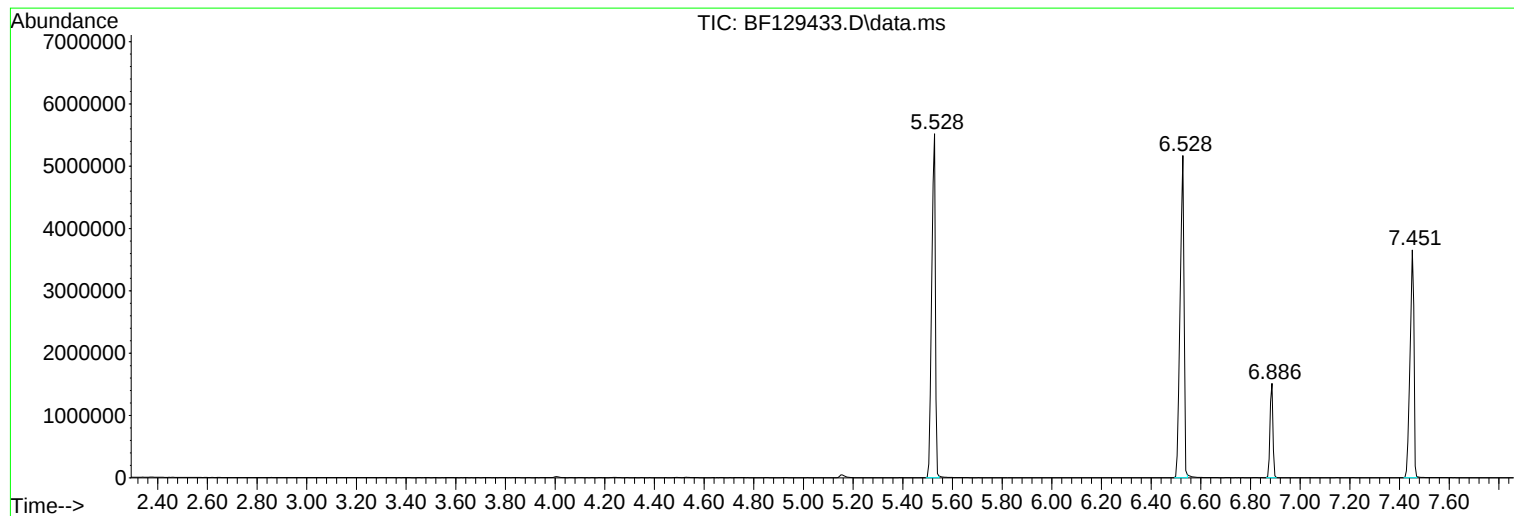

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129433.D
Acq On : 29 Jul 2022 10:13
Operator : CG\JU
Sample : PB146528BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146528BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129433.D
Acq On : 29 Jul 2022 10:13
Operator : CG\JU
Sample : PB146528BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146528BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------