

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
 Data File : BF129462.D
 Acq On : 30 Jul 2022 02:10
 Operator : CG\JU
 Sample : N3896-15 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RVE-72

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	280	284	289	rVB	16067	20274	1.44%	0.155%
2	5.516	545	549	559	rBV	1100750	1068721	75.83%	8.168%
3	6.522	717	720	733	rBV	1251464	1052642	74.69%	8.045%
4	6.881	778	781	785	rBV	1351788	1118834	79.39%	8.551%
5	7.445	873	877	880	rBV	769376	655634	46.52%	5.011%
6	8.169	996	1000	1003	rBV	1563250	1409298	100.00%	10.771%
7	9.239	1178	1182	1185	rBV	1551829	1192871	84.64%	9.117%
8	9.922	1295	1298	1302	rBV	1506062	1354236	96.09%	10.350%
9	10.127	1328	1333	1337	rBV2	12182	16072	1.14%	0.123%
10	10.716	1429	1433	1442	rBV	580763	499319	35.43%	3.816%
11	10.892	1460	1463	1466	rBV	16516	20111	1.43%	0.154%
12	11.416	1548	1552	1555	rBV	1359350	1132106	80.33%	8.652%
13	11.439	1555	1556	1560	rVV	116424	68891	4.89%	0.527%
14	11.492	1560	1565	1568	rVB	22105	24878	1.77%	0.190%
15	11.651	1587	1592	1595	rBV3	12236	15596	1.11%	0.119%
16	11.792	1614	1616	1620	rVB	31757	26352	1.87%	0.201%
17	11.916	1633	1637	1640	rBV	15942	19216	1.36%	0.147%
18	12.027	1653	1656	1659	rBV	17175	19011	1.35%	0.145%
19	12.210	1683	1687	1690	rBV4	13092	15753	1.12%	0.120%
20	12.468	1728	1731	1733	rBV4	11572	15260	1.08%	0.117%
21	12.633	1755	1759	1764	rBV	125462	116859	8.29%	0.893%
22	12.863	1791	1798	1801	rBV	122526	130850	9.28%	1.000%
23	12.998	1817	1821	1824	rBV	1157741	910405	64.60%	6.958%
24	14.062	1997	2002	2005	rBV	1305789	1196041	84.87%	9.141%
25	14.151	2015	2017	2022	rVB2	47643	57221	4.06%	0.437%
26	15.557	2251	2256	2261	rBV	727155	928068	65.85%	7.093%




Sum of corrected areas: 13084519

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129462.D
Acq On : 30 Jul 2022 02:10
Operator : CG\JU
Sample : N3896-15 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

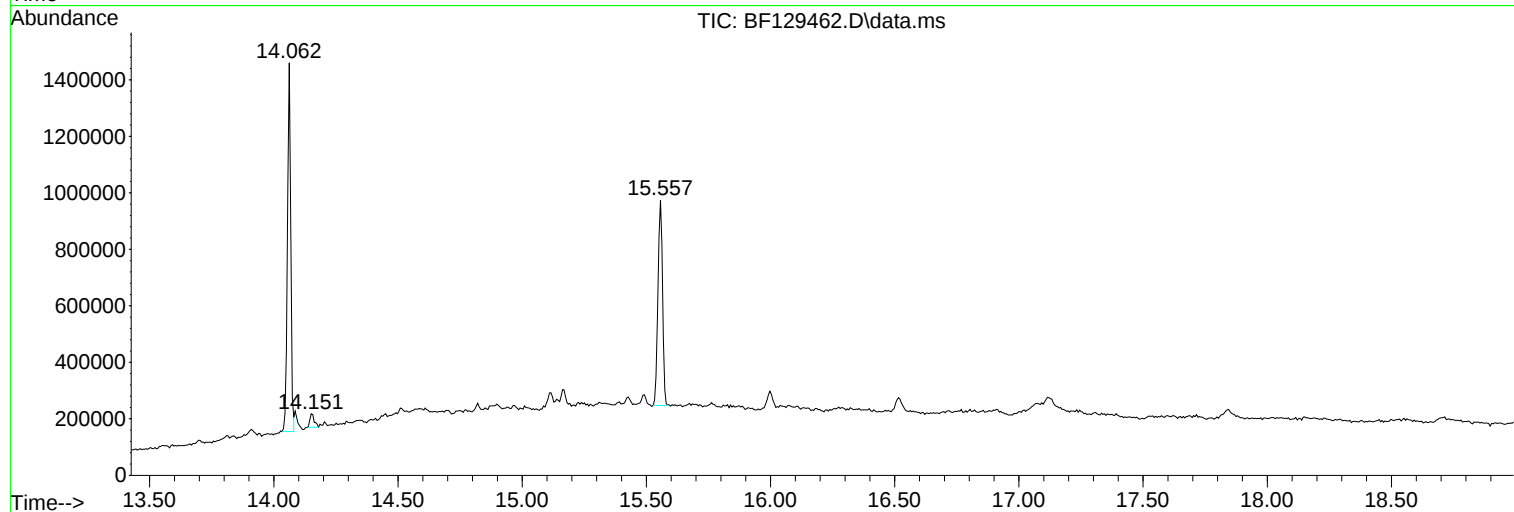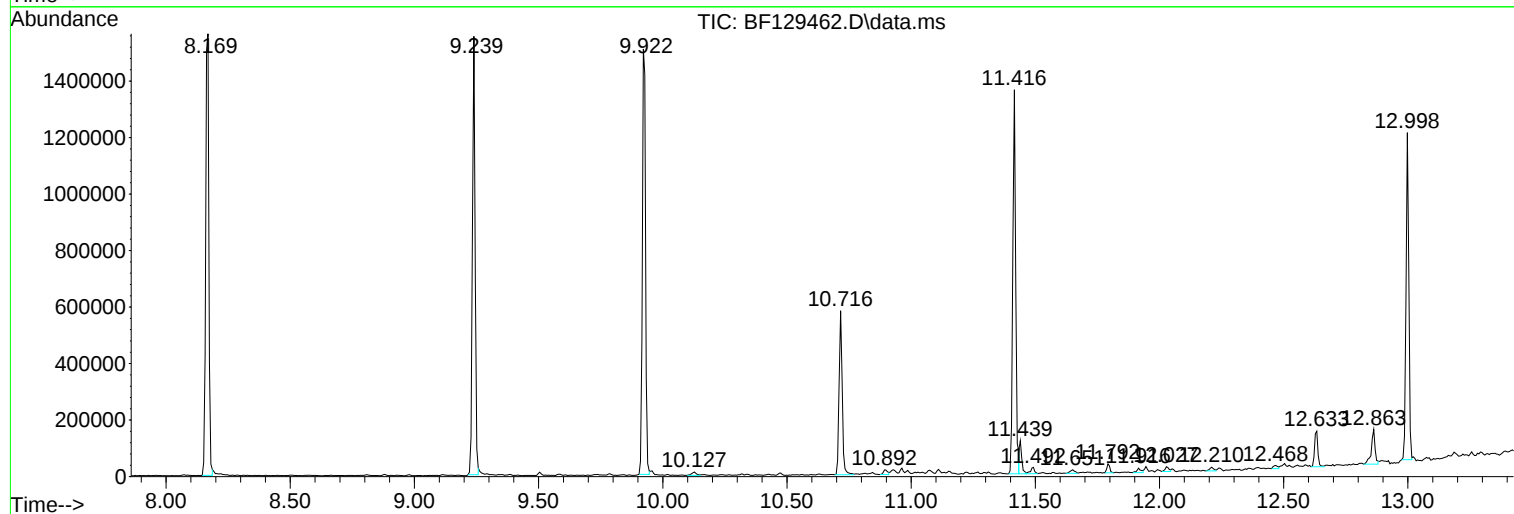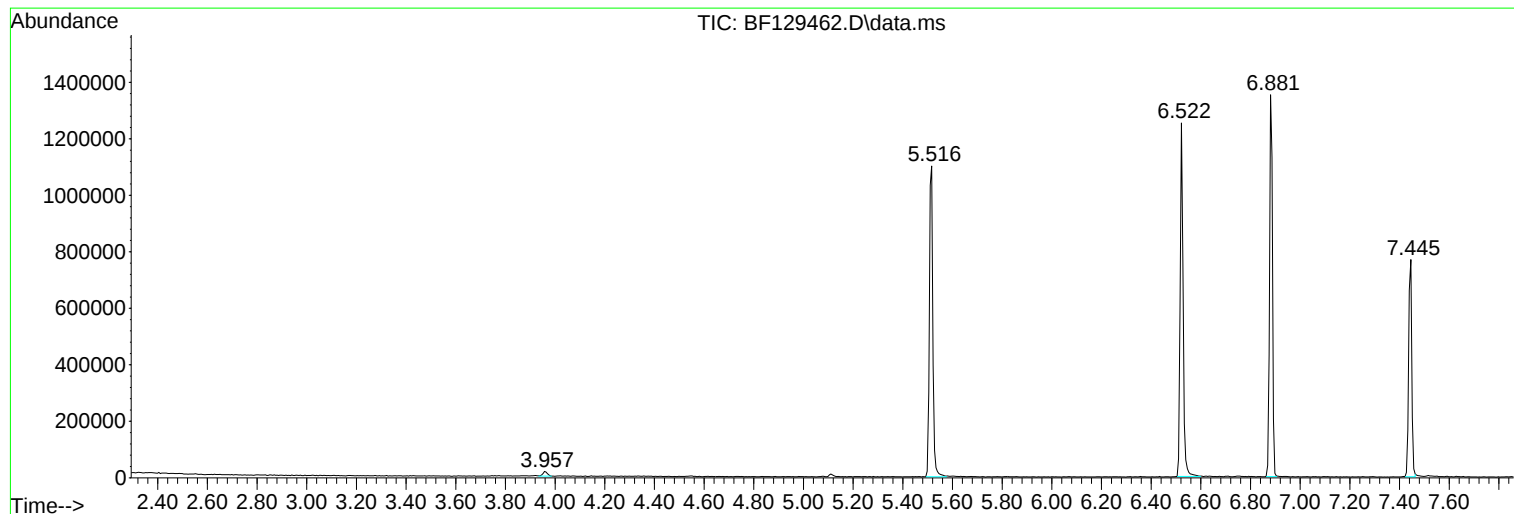

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129462.D
Acq On : 30 Jul 2022 02:10
Operator : CG\JU
Sample : N3896-15 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129462.D
Acq On : 30 Jul 2022 02:10
Operator : CG\JU
Sample : N3896-15 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------