


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
 Data File : BF129442.D
 Acq On : 29 Jul 2022 15:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 17:24:17 2022

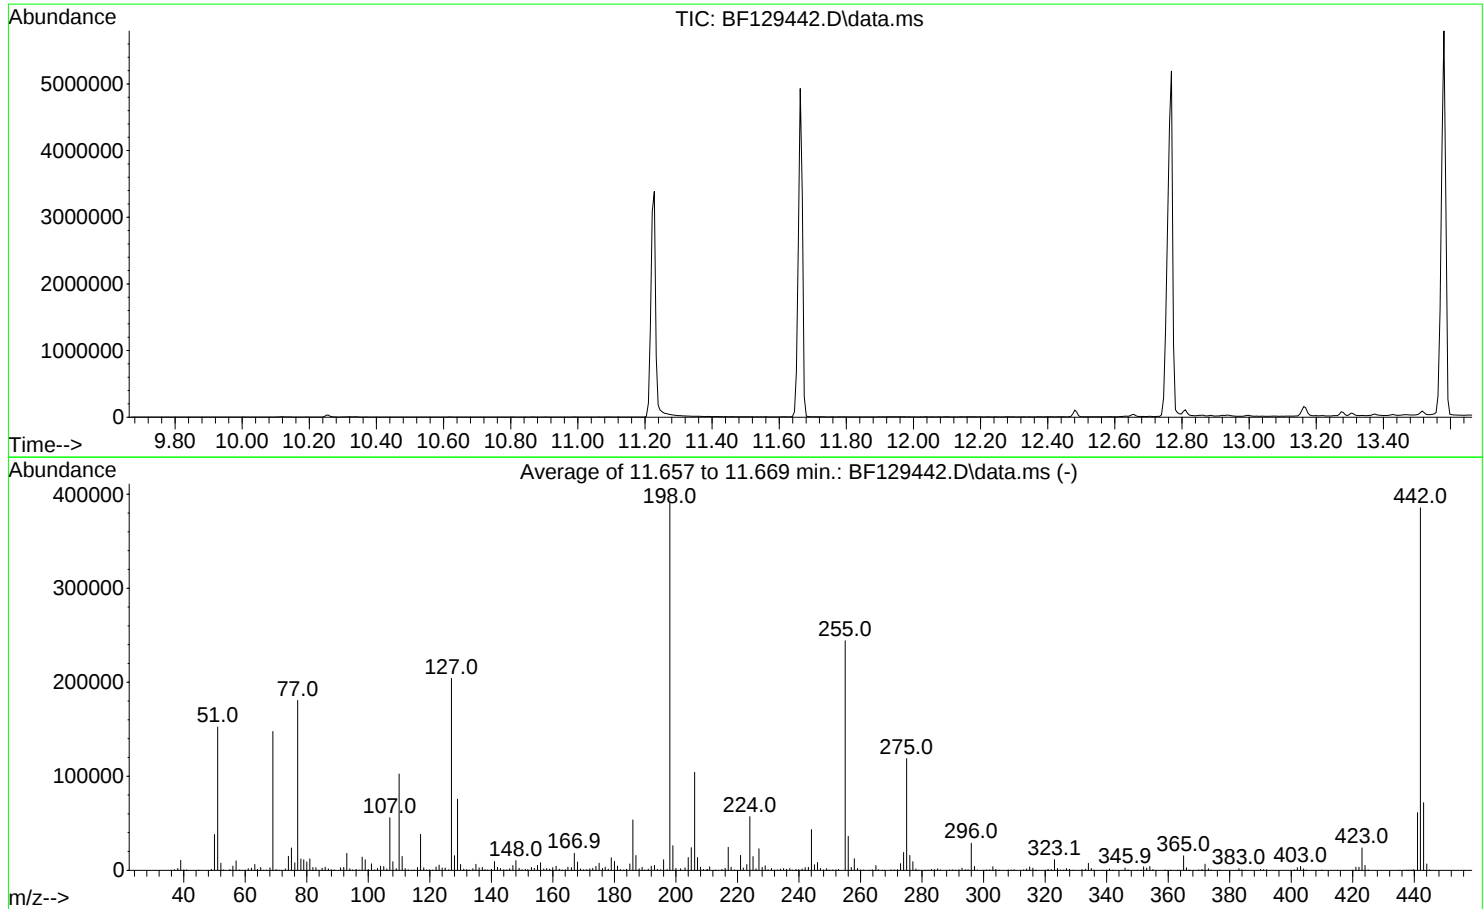




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	152341	PASS
68	69	0.00	2	1.7	2560	PASS
69	198	0.00	100	37.7	147701	PASS
70	69	0.00	2	0.6	855	PASS
127	198	10	80	52.2	204224	PASS
197	198	0.00	2	0.2	808	PASS
198	198	100	100	100.0	391275	PASS
199	198	5	9	6.7	26133	PASS
275	198	10	60	30.4	118795	PASS
365	198	1	100	3.9	15350	PASS
441	198	0.01	100	15.7	61320	PASS
442	442	50	100	100.0	385557	PASS
443	442	15	24	18.7	71941	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129442.D
Acq On : 29 Jul 2022 15:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 18:55:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

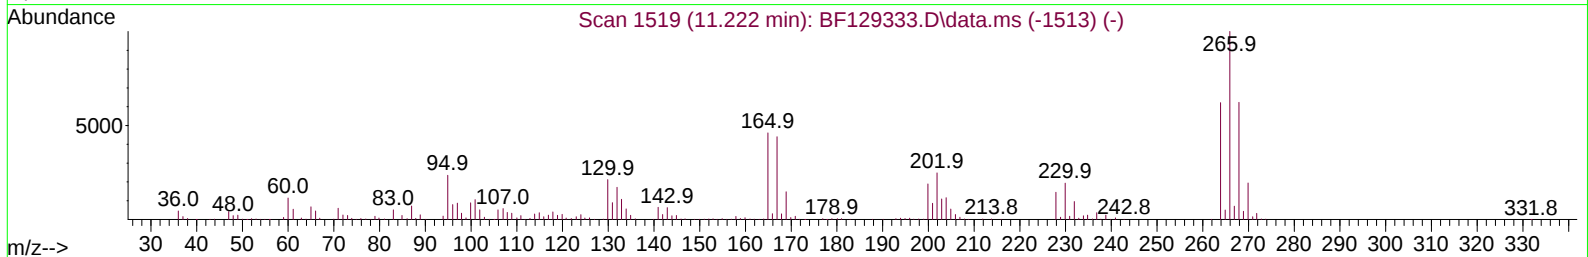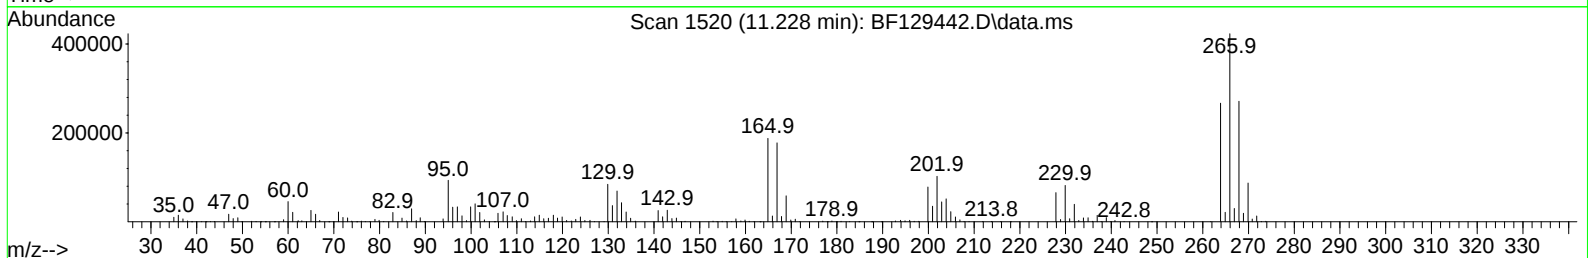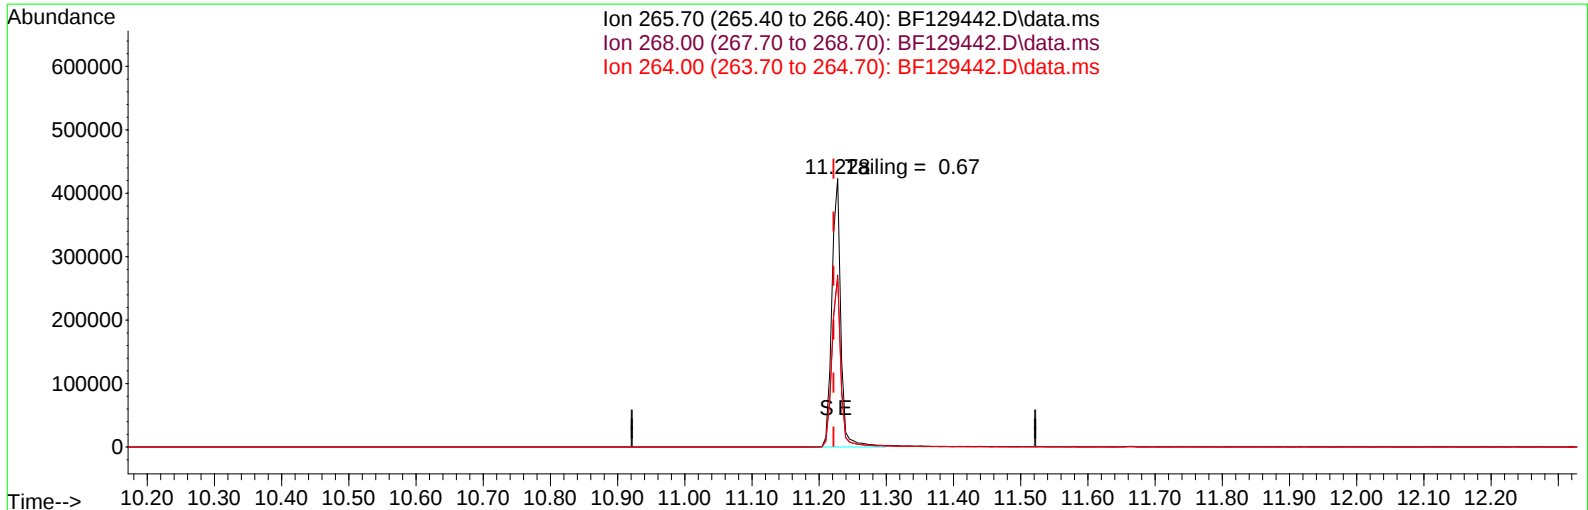

TIC: BF129442.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.006) 829663.31 ng




response 396009

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.12
264.00	61.80	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072922\
Data File : BF129442.D
Acq On : 29 Jul 2022 15:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 18:55:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

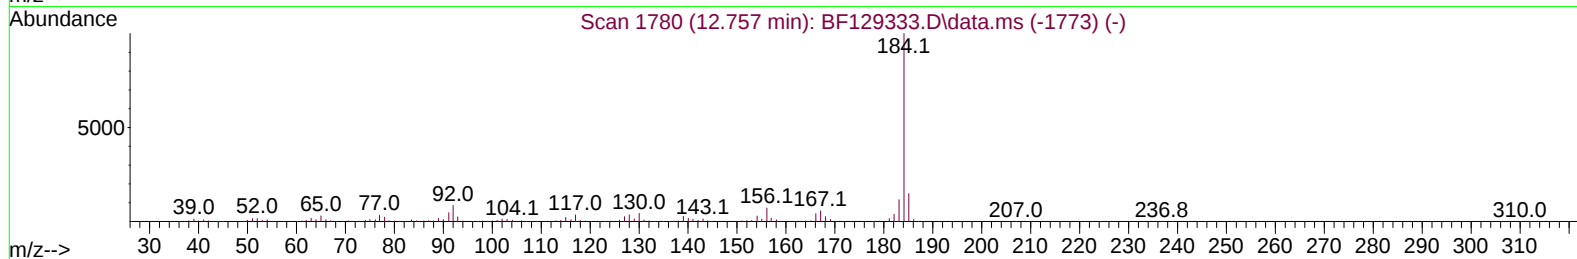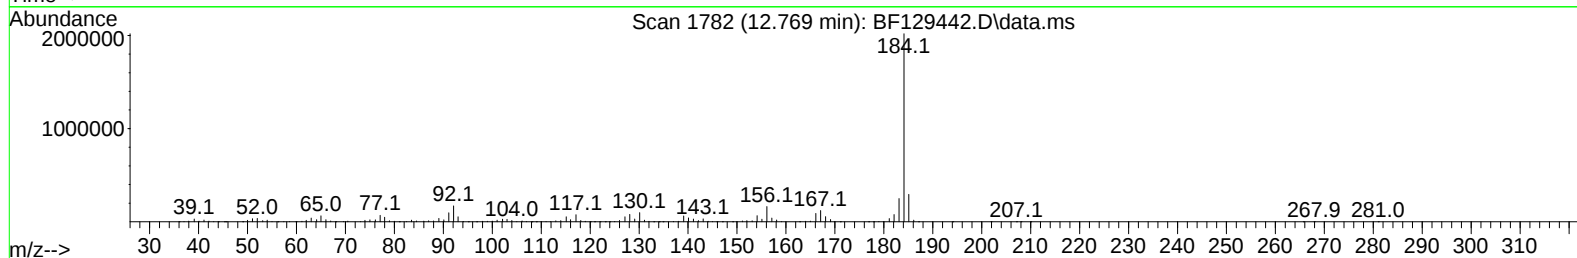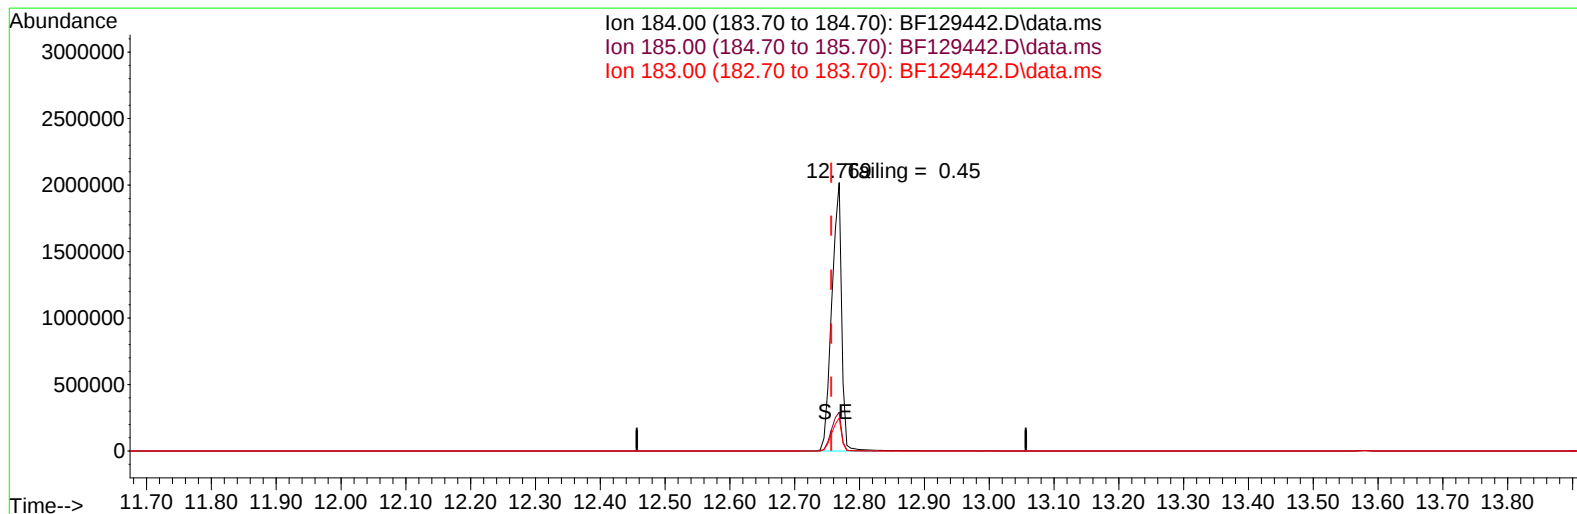

TIC: BF129442.D\data.ms

(77) Benzidine

12.769min (+ 0.012) 73265.41 ng

response 2132747

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.53
183.00	11.60	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/29/2022	BNA_F	<u>BF129442.D</u>
Compound Name	Response	Retention Time
DDT	1010754	13.58
DDD	10087	13.27
DDE	1752	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11839	1022593	1.16

Instrument :
BNA_F
ClientSampleId :
DFTPP