



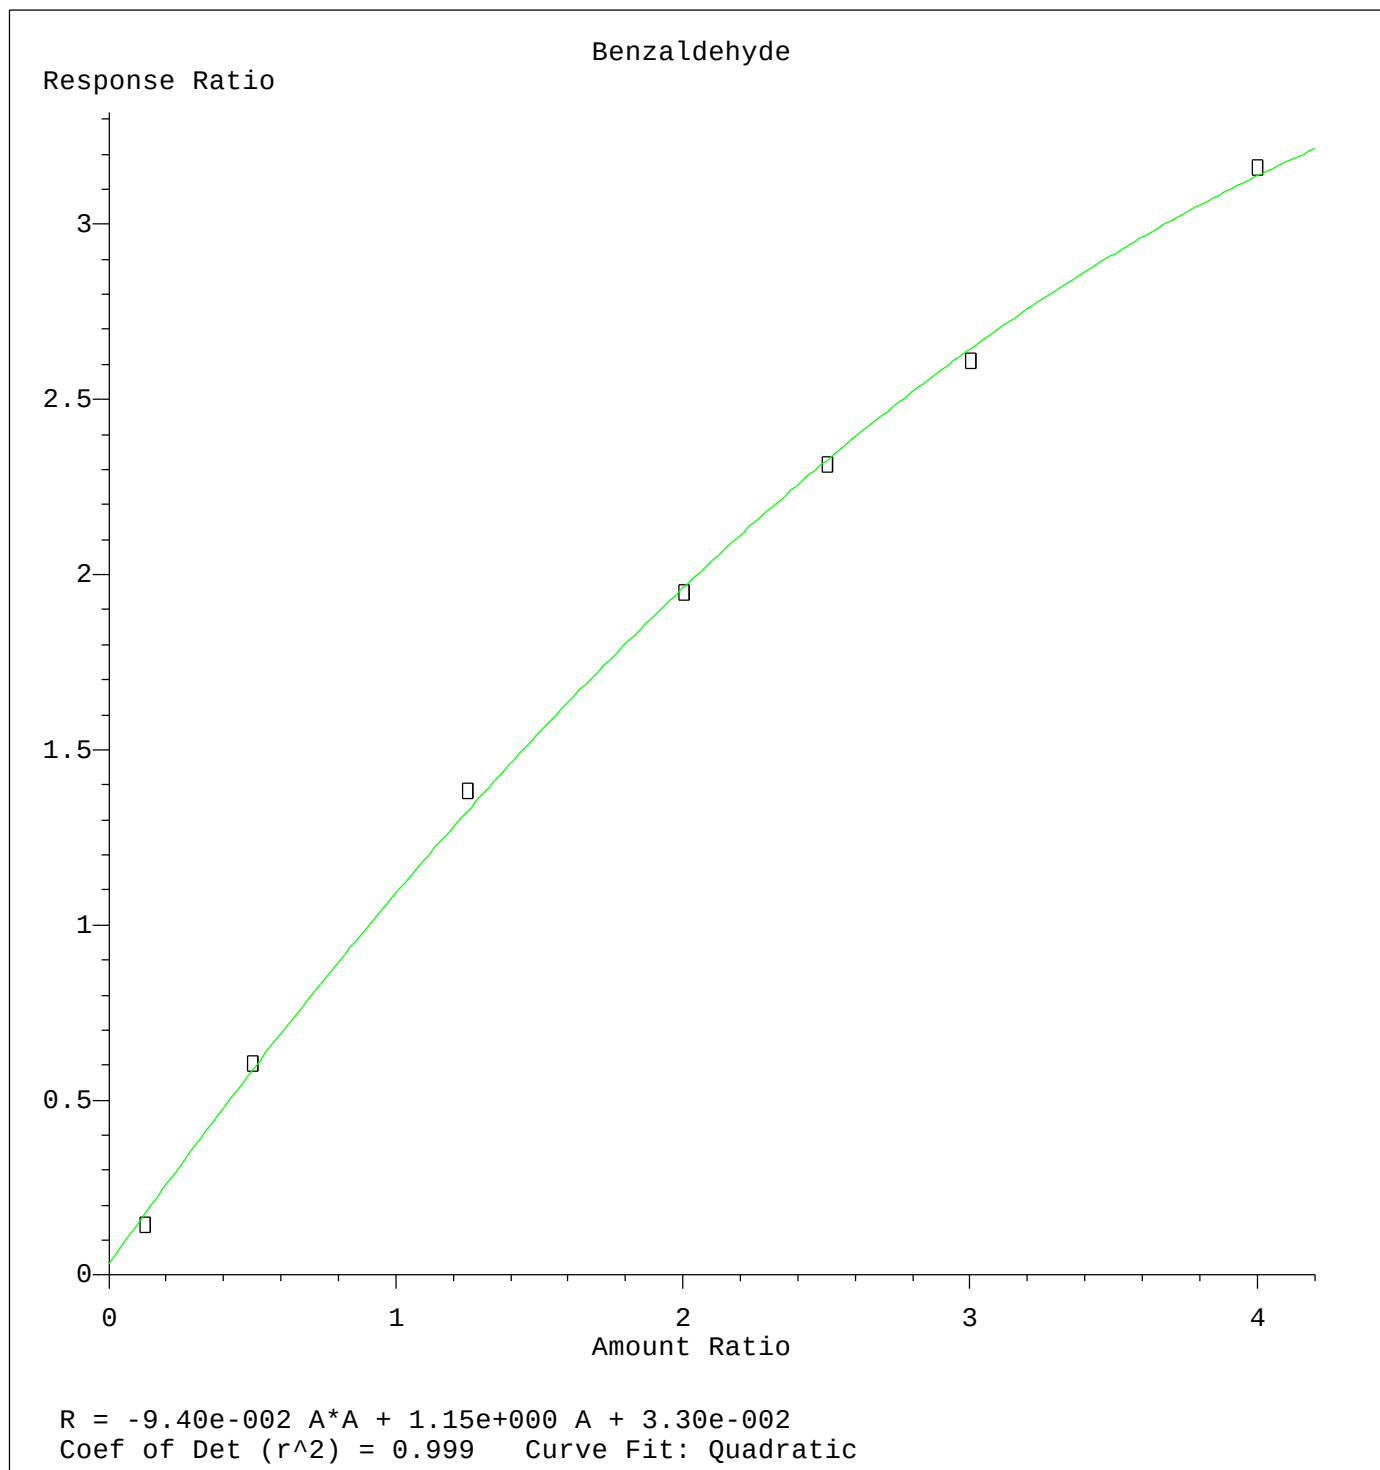


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015

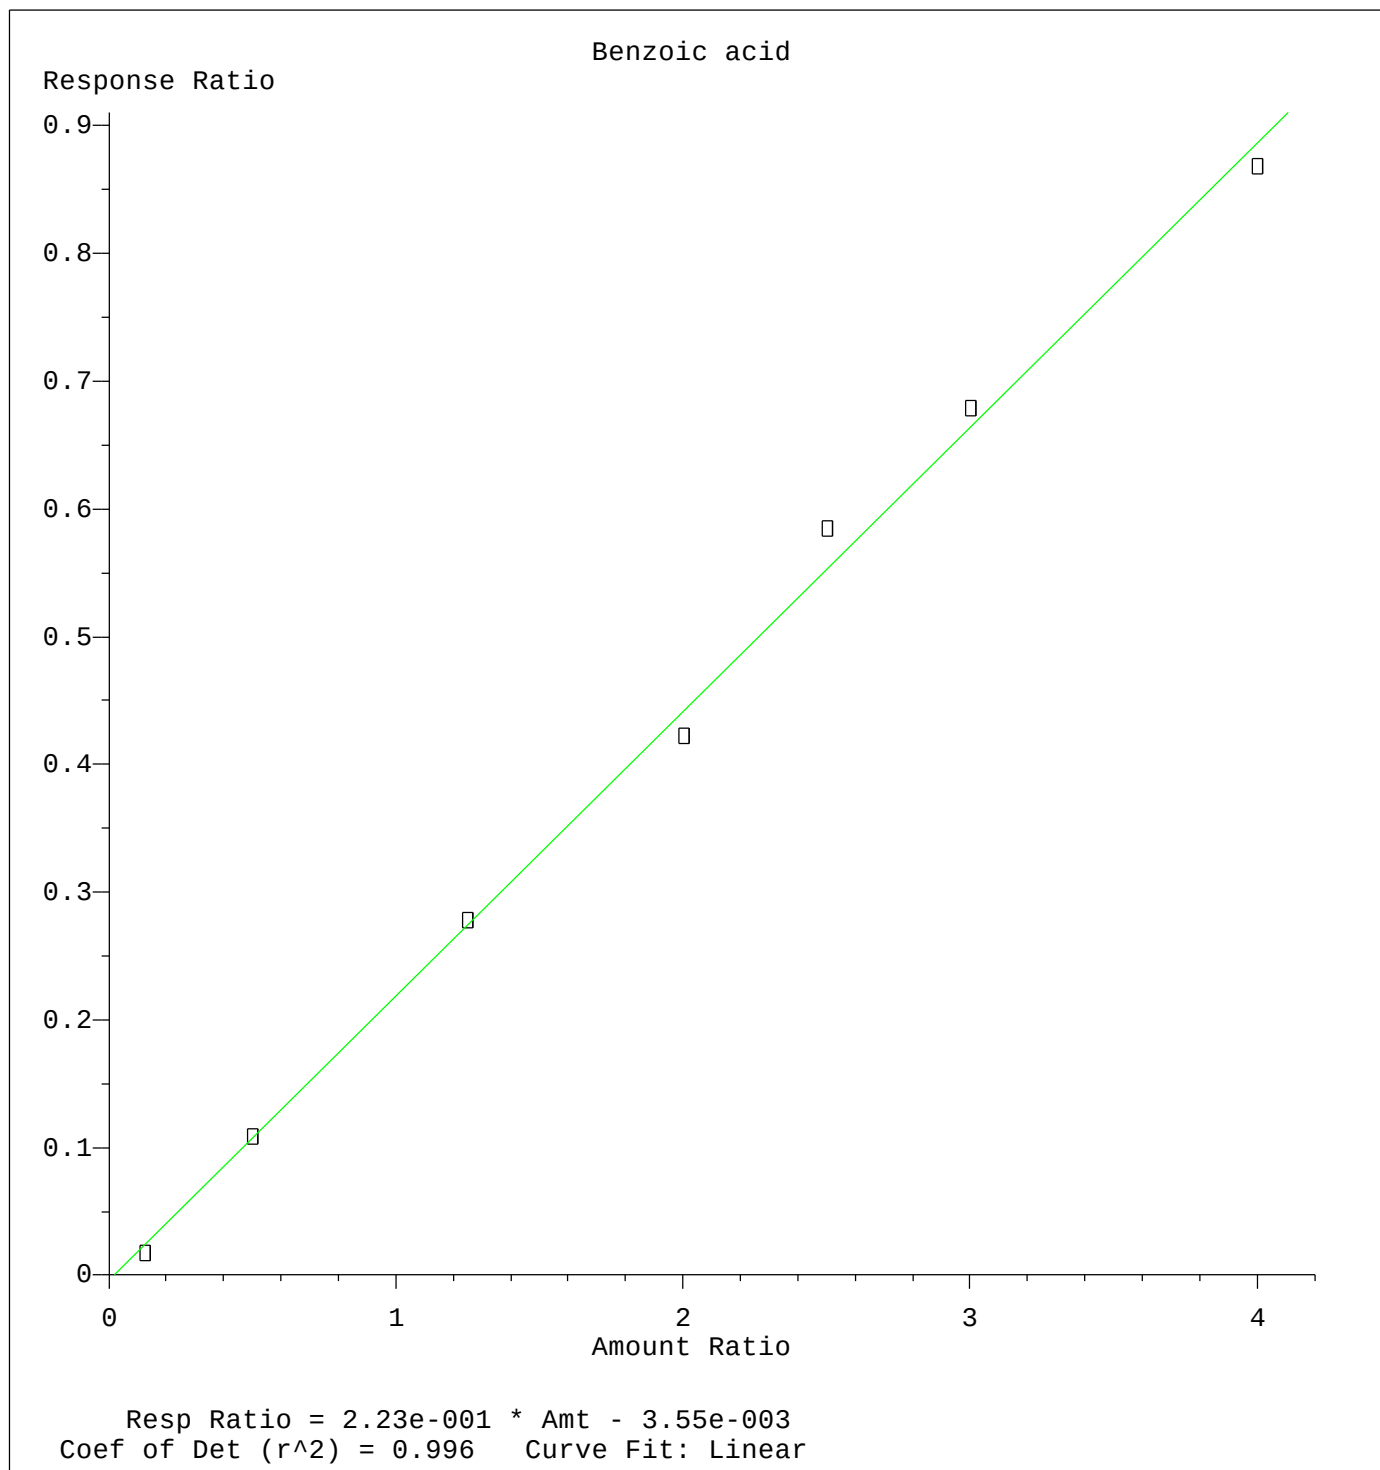

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015


4-Chlorophenyl-phenylether

Response Ratio

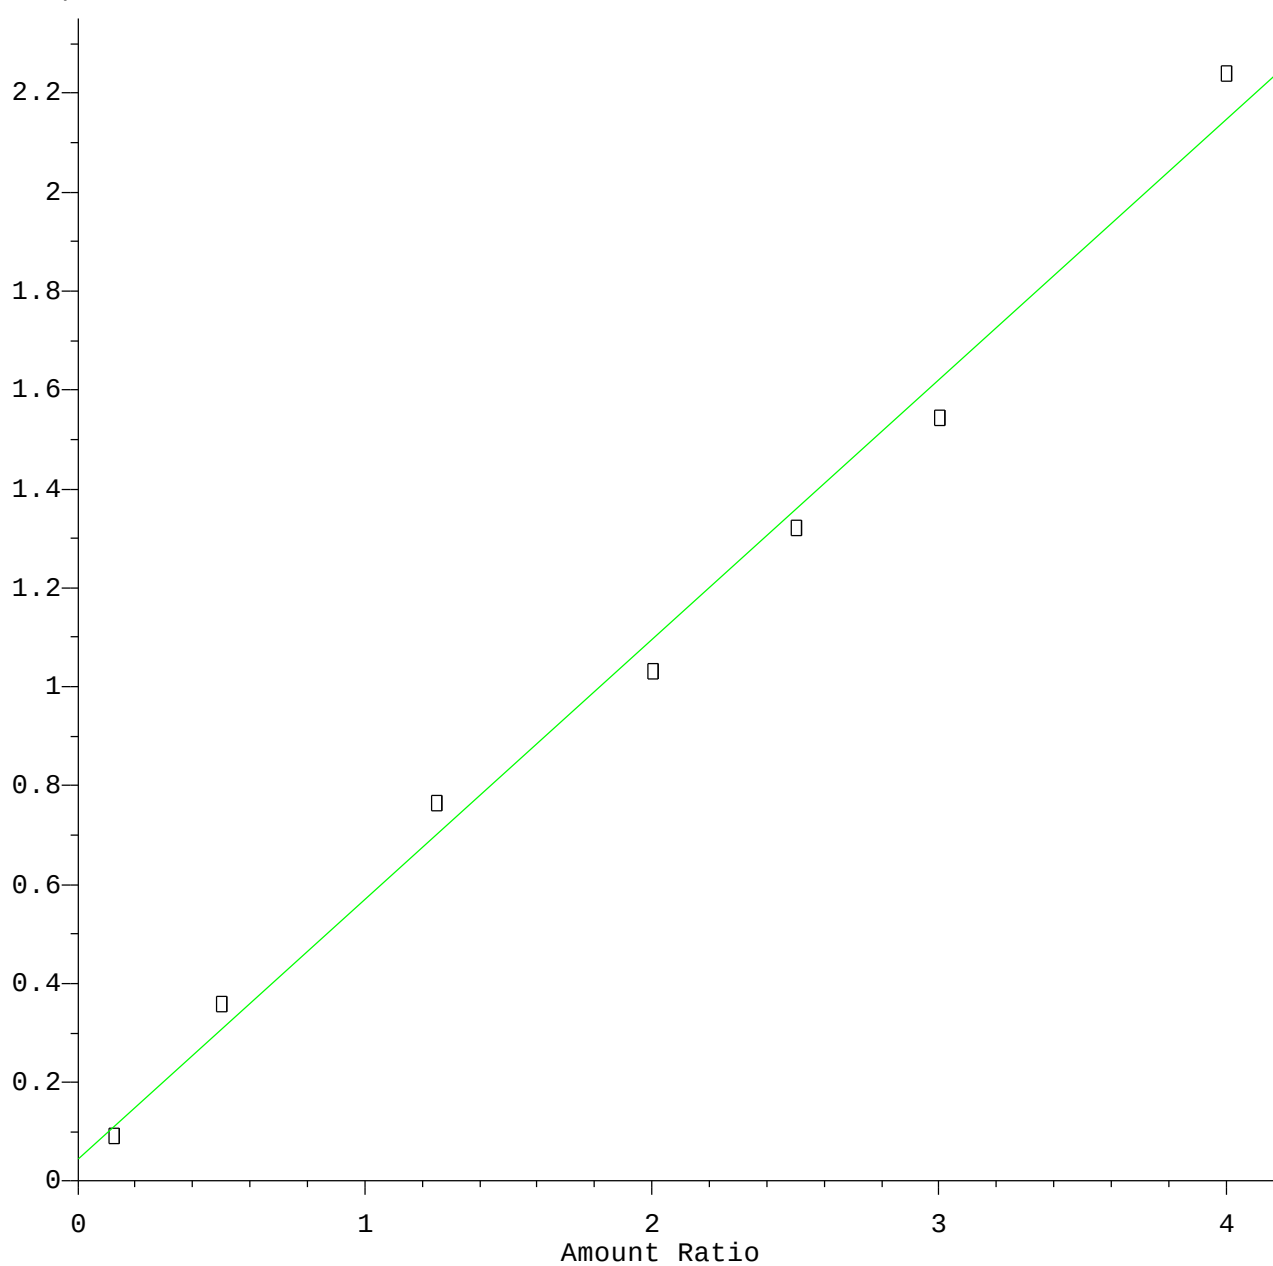


Resp Ratio = $5.26 \times 10^{-1} \times \text{Amt} + 4.44 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015

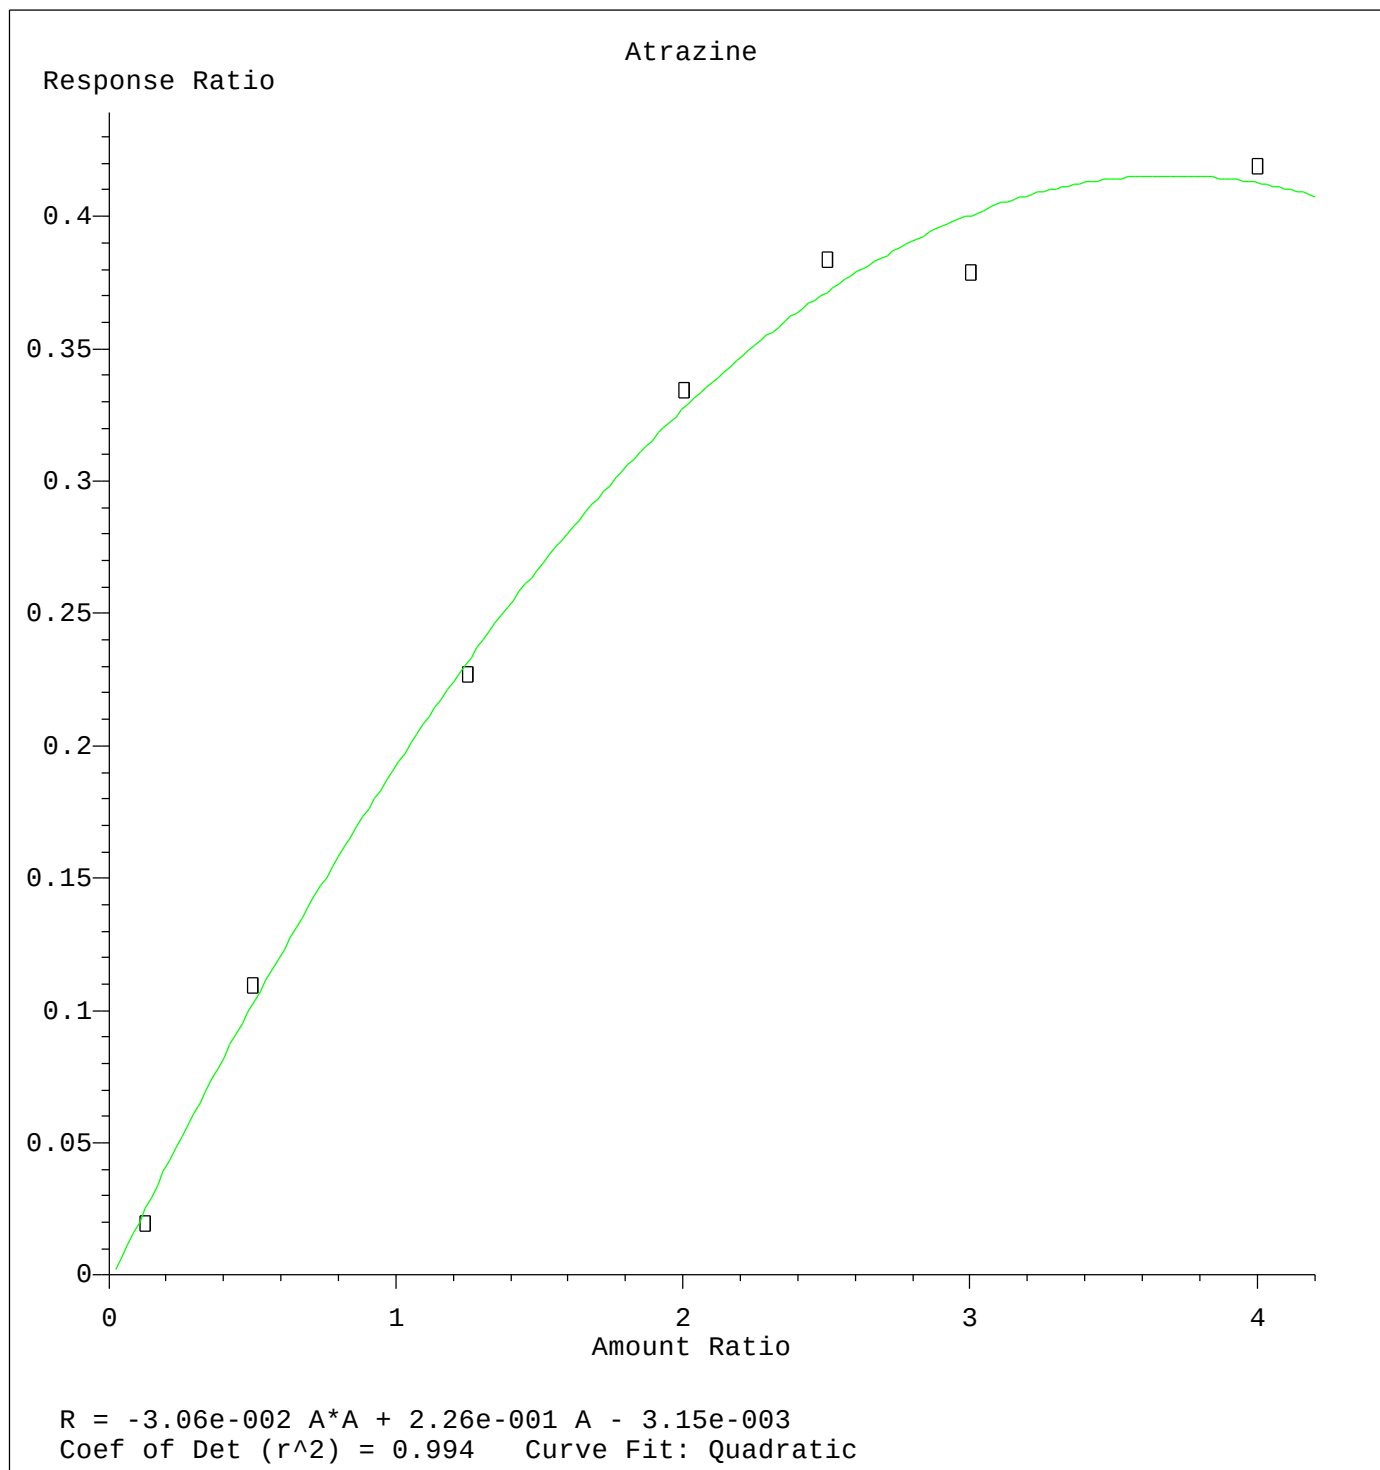

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015

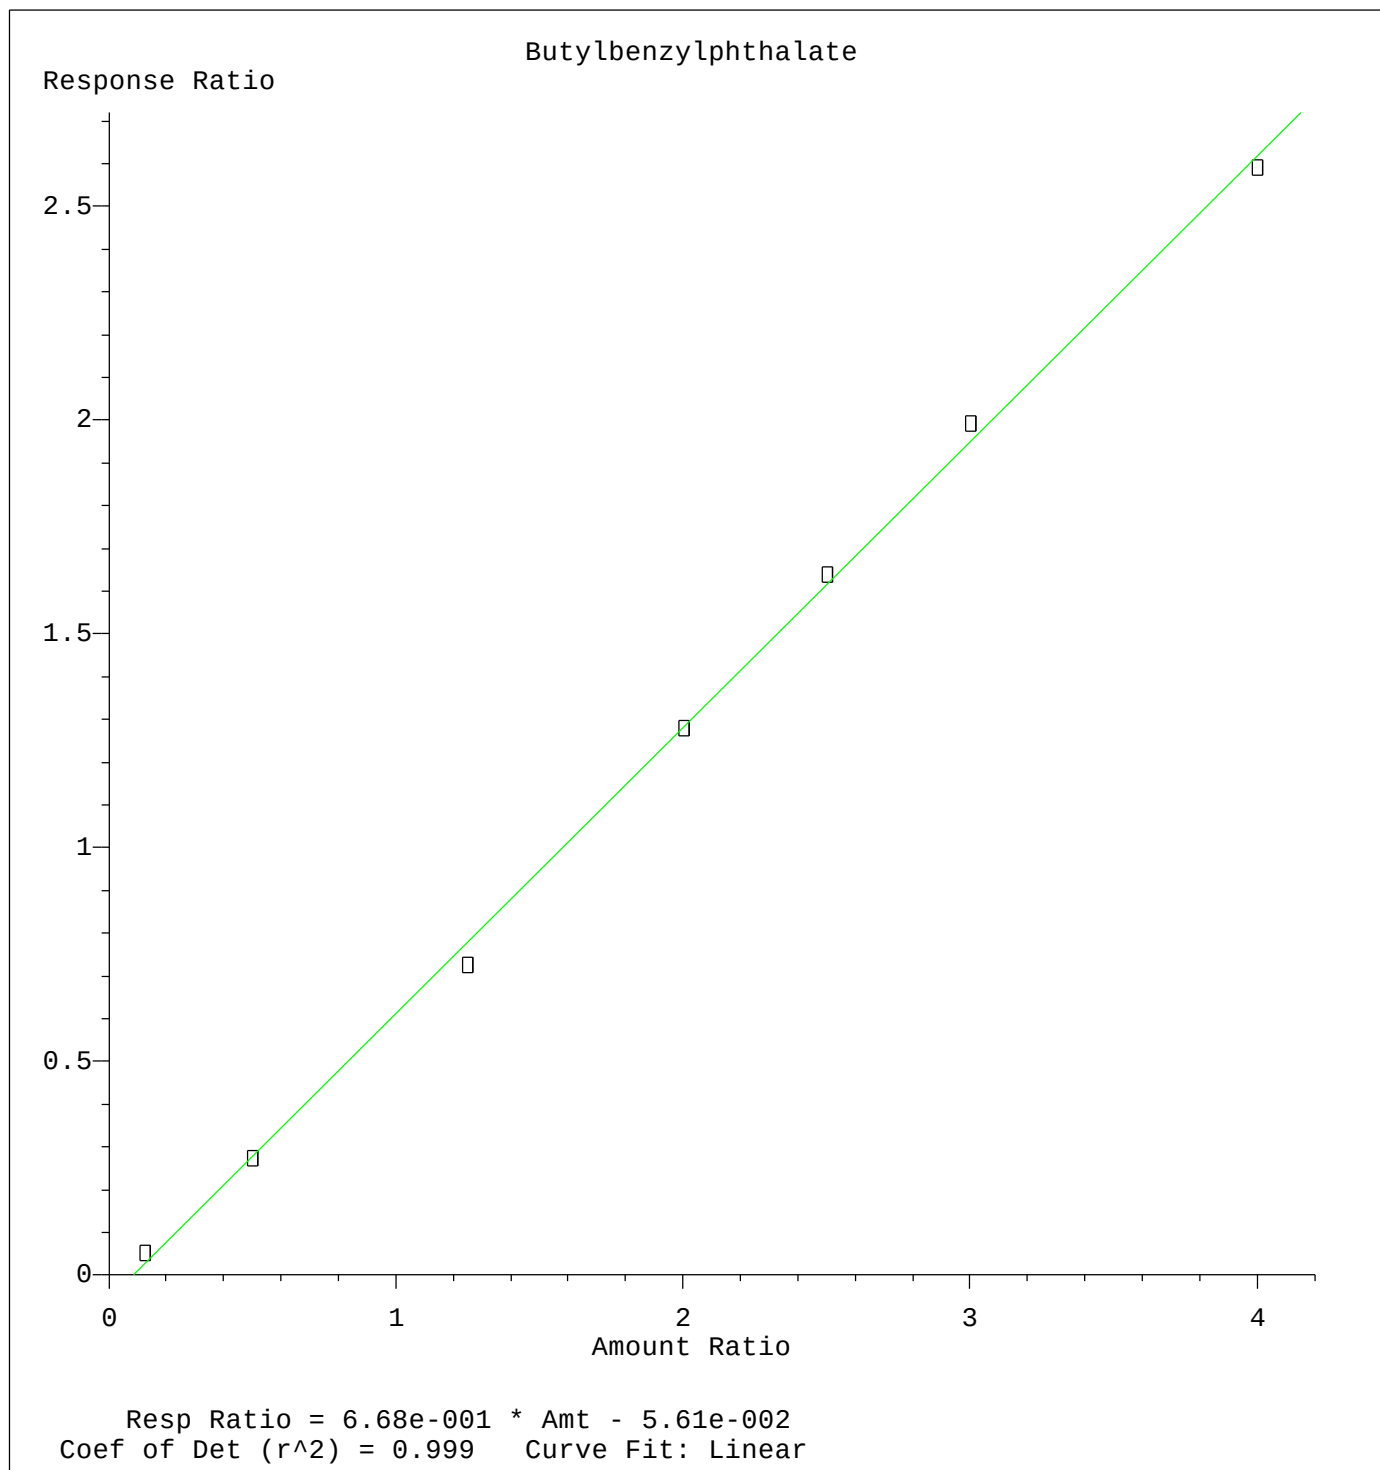

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015

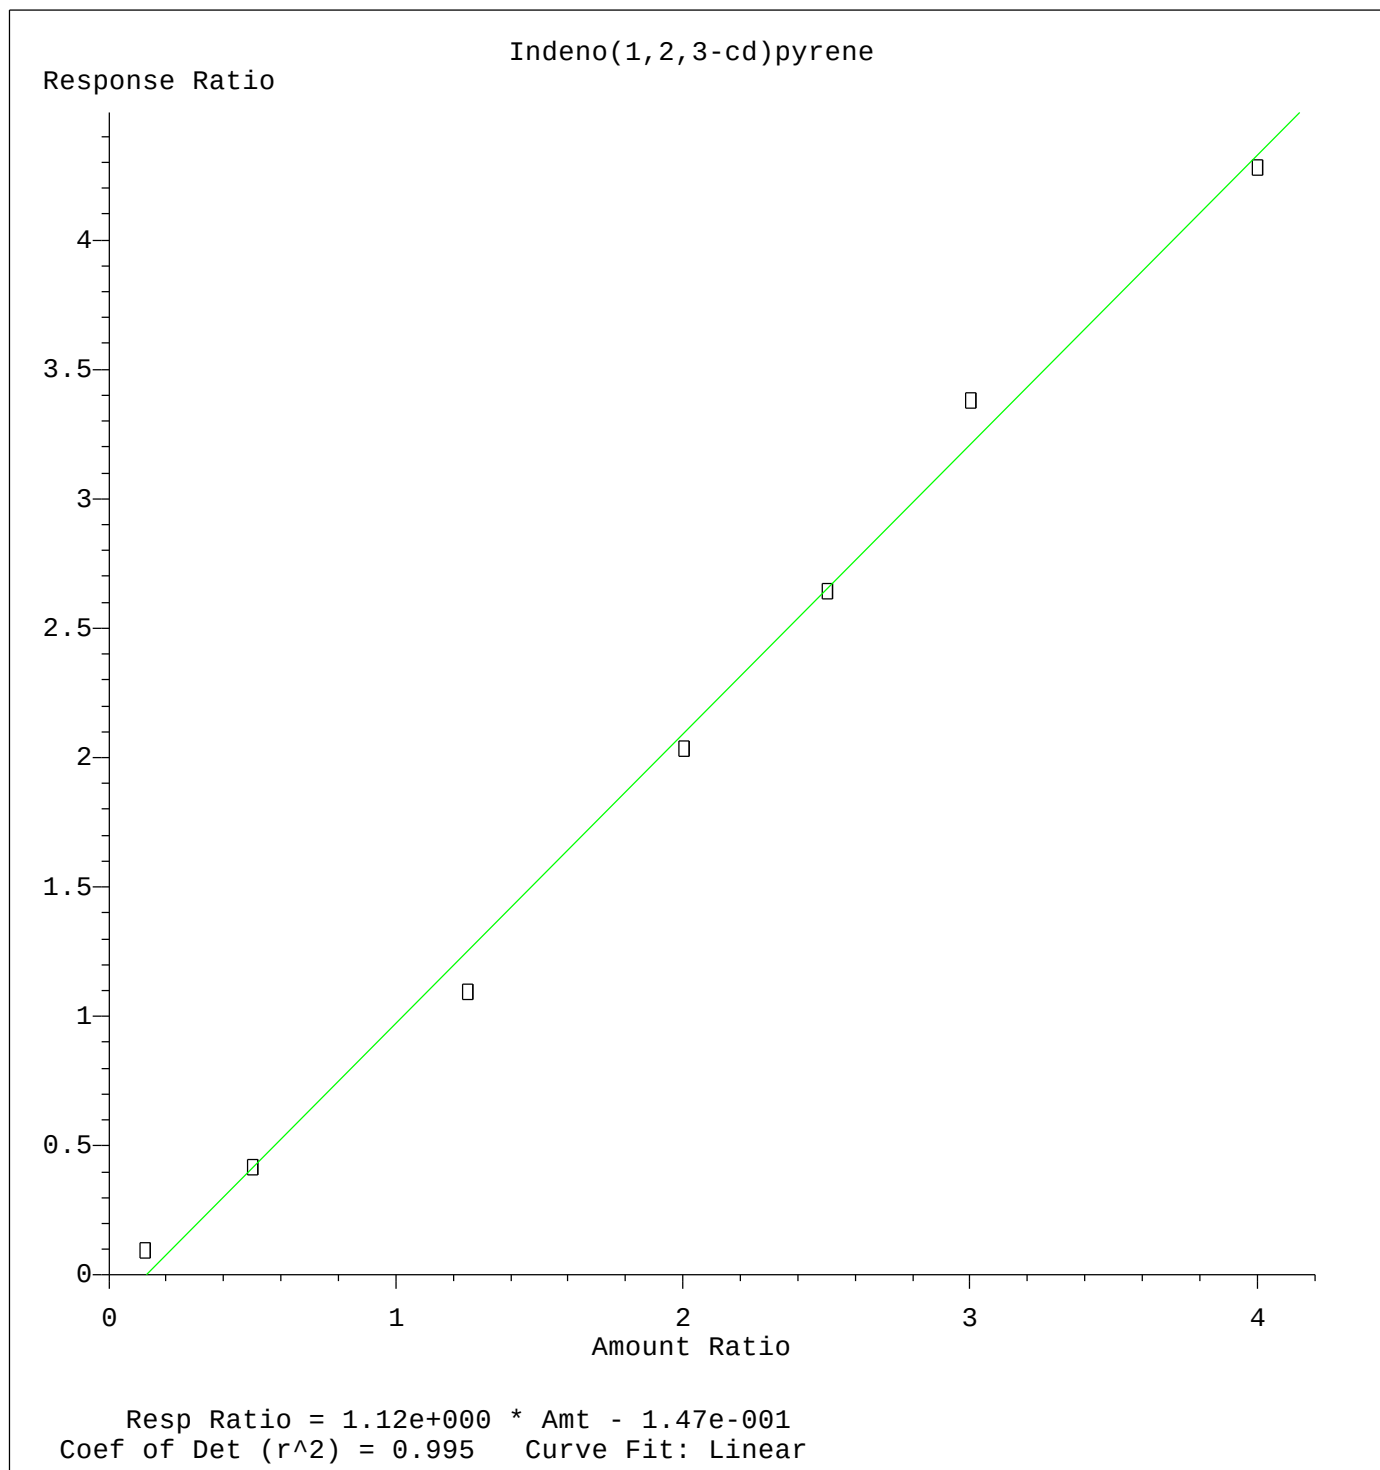

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Calibration Table Last Updated: Fri Jul 31 01:45:22 2015