


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073015\
 Data File : BF080700.D
 Acq On : 30 Jul 2015 14:12
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 31 01:45:22 2015

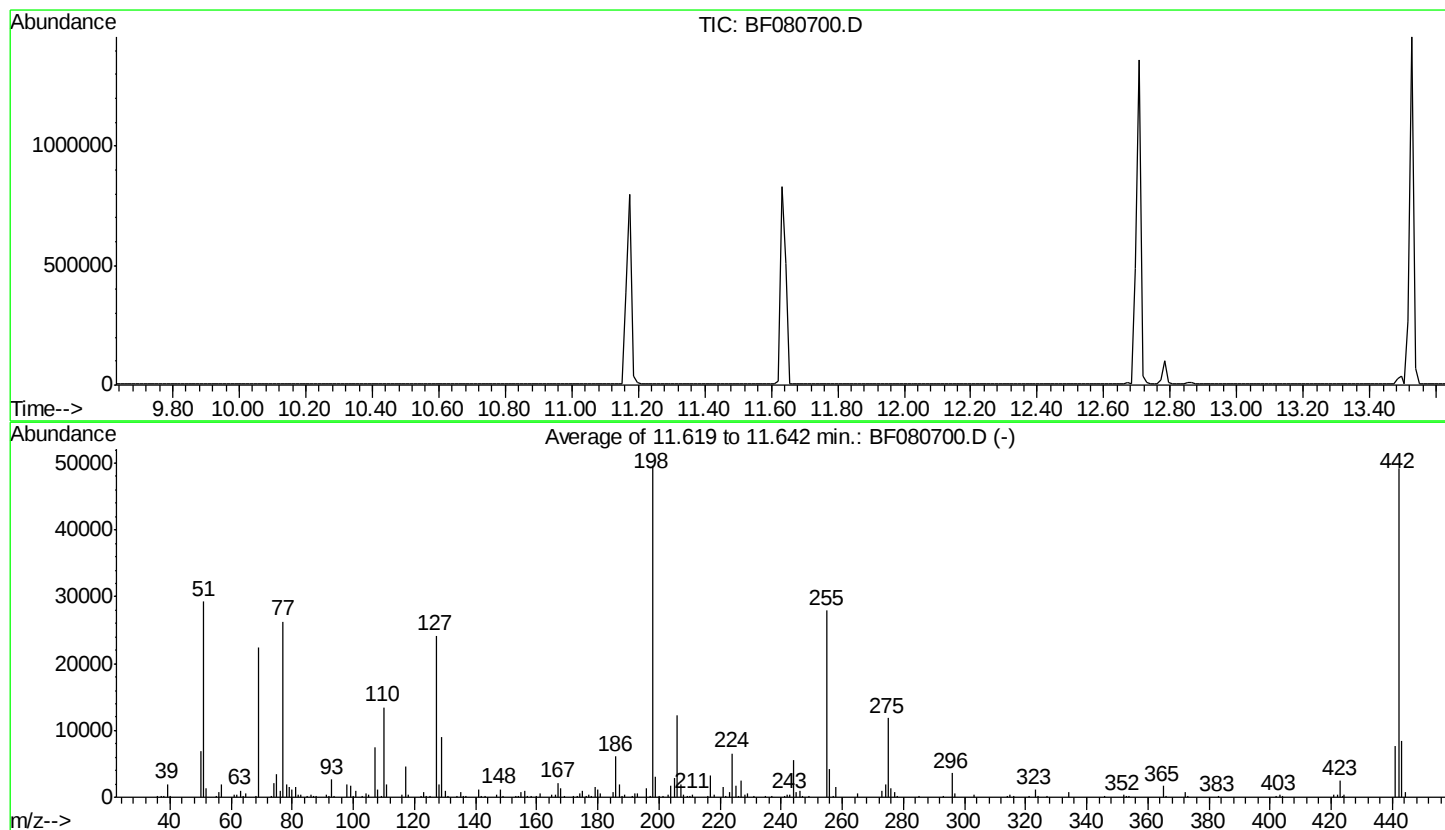

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	29221	PASS
68	69	0.00	2	1.0	231	PASS
69	198	0.00	100	45.2	22424	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	24217	PASS
197	198	0.00	2	0.4	214	PASS
198	198	100	100	100.0	49622	PASS
199	198	5	9	6.2	3094	PASS
275	198	10	60	23.9	11862	PASS
365	198	1	100	3.4	1684	PASS
441	442	0.01	24	15.7	7735	PASS
442	198	50	100	99.2	49220	PASS
443	442	15	24	17.3	8530	PASS