


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073015\
 Data File : BF080709.D
 Acq On : 30 Jul 2015 23:52
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 31 01:45:22 2015

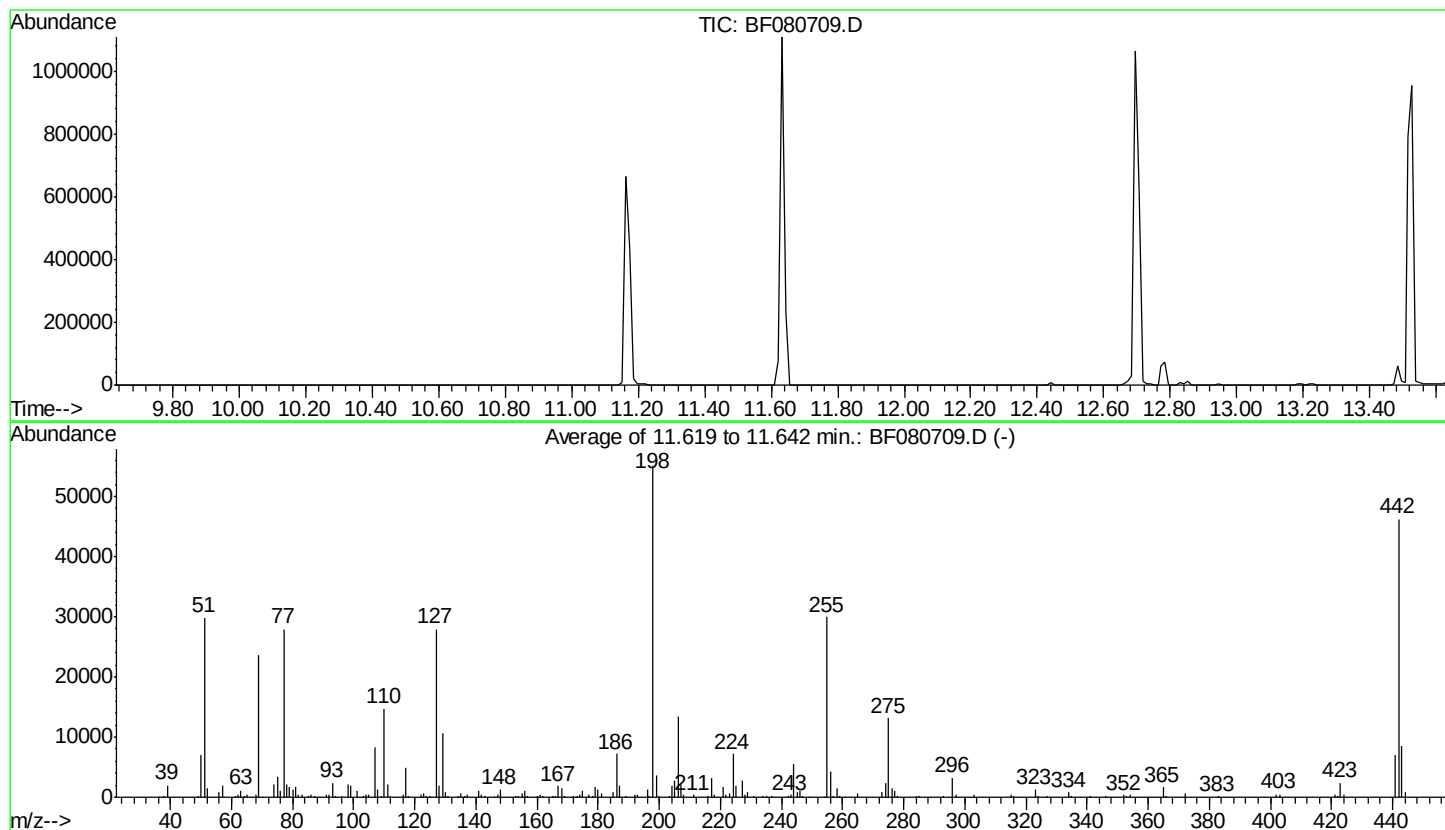

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	29883	PASS
68	69	0.00	2	1.4	338	PASS
69	198	0.00	100	42.7	23524	PASS
70	69	0.00	2	0.5	107	PASS
127	198	10	80	50.7	27938	PASS
197	198	0.00	2	0.5	286	PASS
198	198	100	100	100.0	55106	PASS
199	198	5	9	6.5	3571	PASS
275	198	10	60	23.9	13182	PASS
365	198	1	100	3.1	1681	PASS
441	442	0.01	24	15.1	6953	PASS
442	198	50	100	83.8	46186	PASS
443	442	15	24	18.5	8554	PASS