
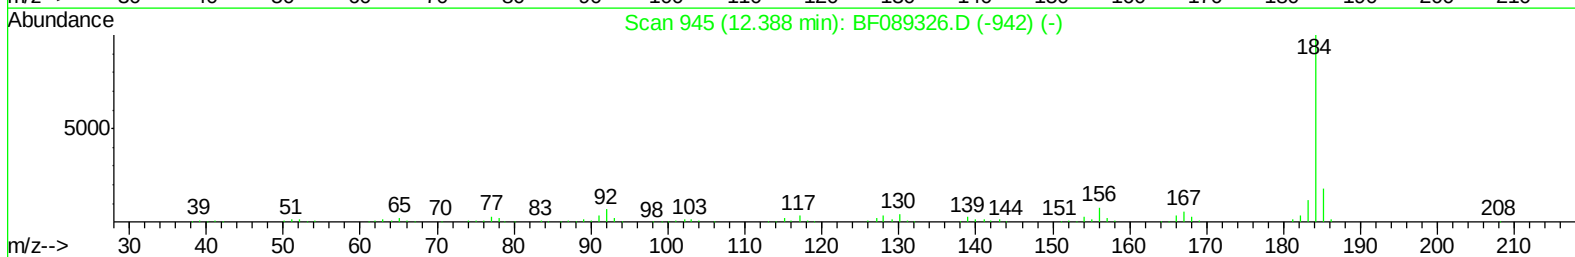
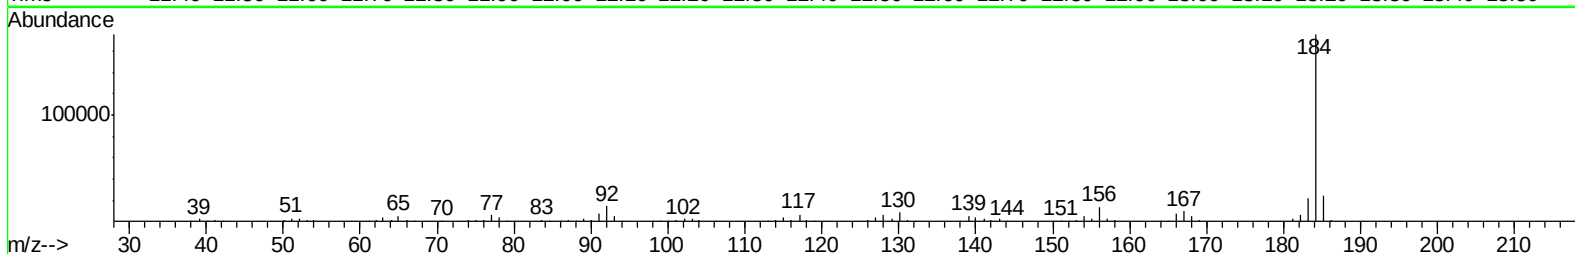


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073016\
Data File : BF089414.D
Acq On : 29 Jul 2016 17:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 05:49:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 30 01:00:15 2016
Response via : Initial Calibration

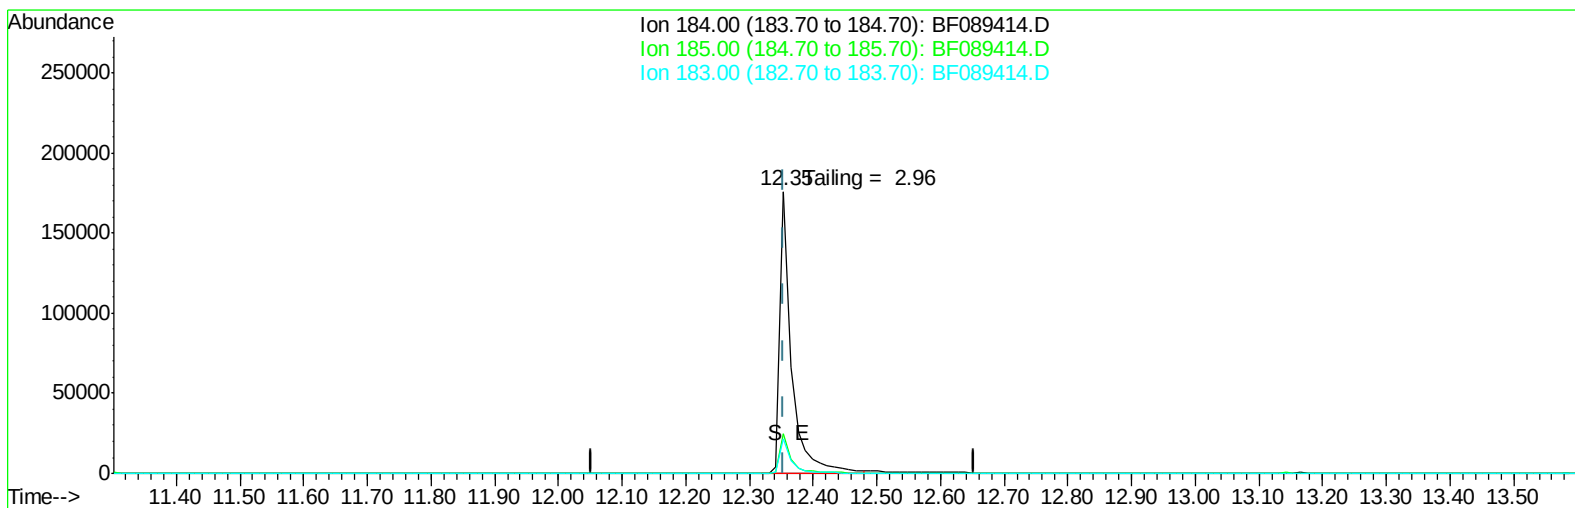

TIC: BF089414.D

(76) Benzidine




12.354min (-0.000) 0.00ng

response 225510

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	13.90
183.00	12.20	12.35
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073016\  
Data File : BF089414.D  
Acq On    : 29 Jul 2016   17:01  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jul 30 05:49:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 30 01:00:15 2016
Response via : Initial Calibration

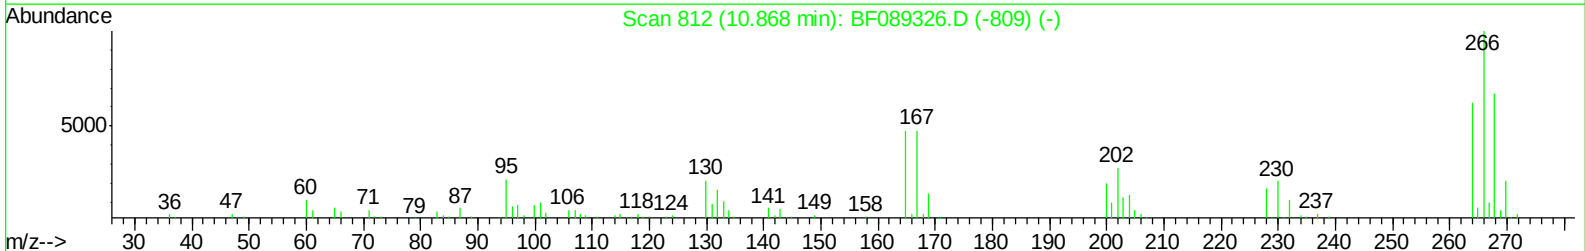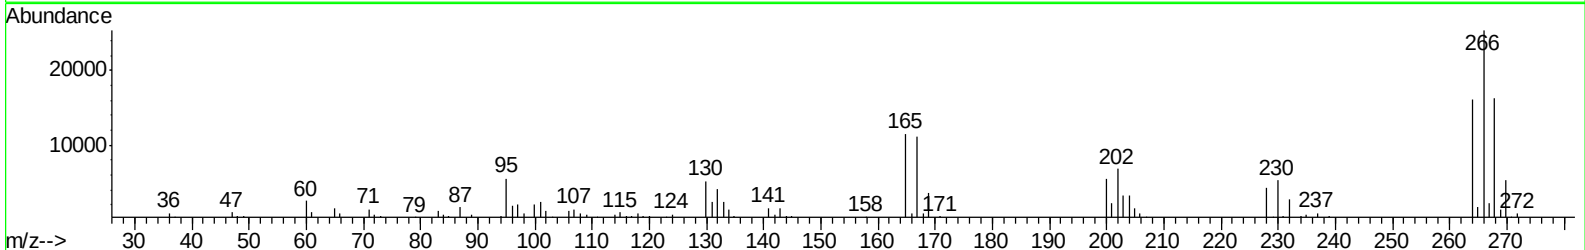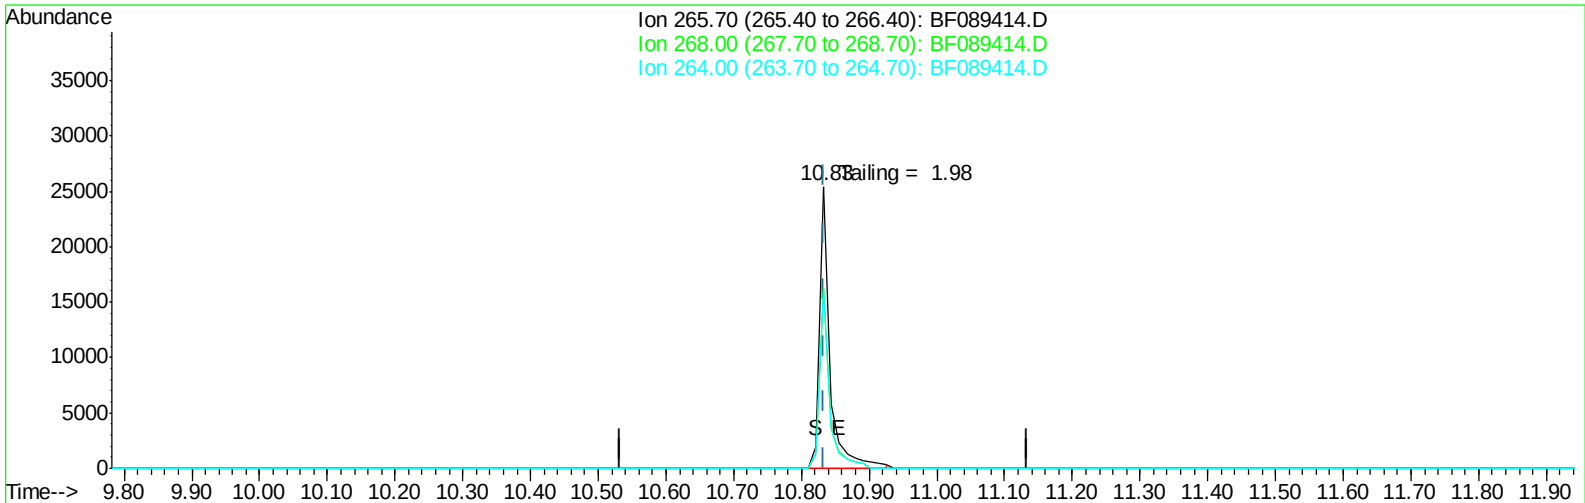

TIC: BF089414.D

(69) Pentachlorophenol (C)

10.833min (-0.000) 0.00ng

response 27139