
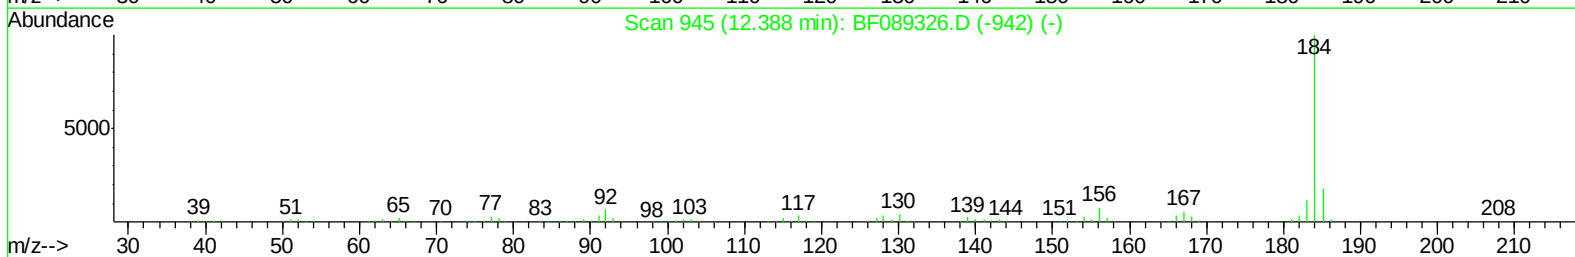
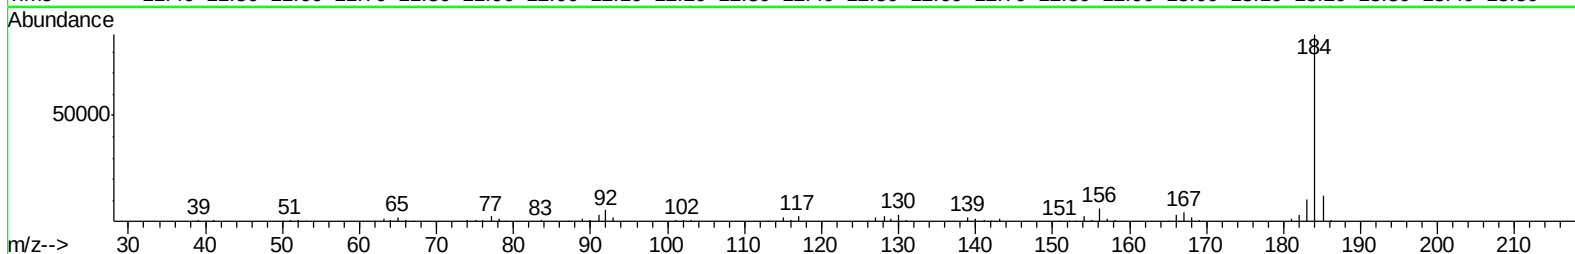


Data Path : Z:\HPCHEM1\BNA F\Data\BF073016\
Data File : BF089438.D
Acq On : 31 Jul 2016 23:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:11:39 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

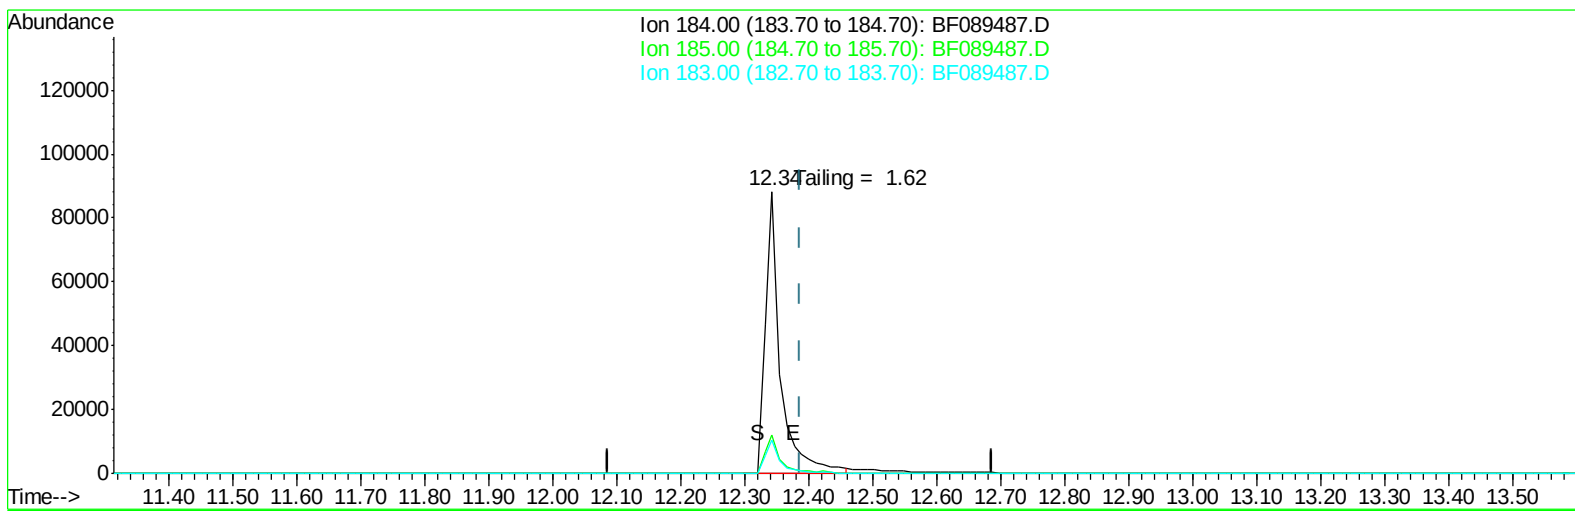

TIC: BF089487.D

(76) Benzidine




12.342min (-0.045) 0.00ng

response 151495

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	13.76
183.00	12.20	11.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF073016\
Data File : BF089438.D
Acq On : 31 Jul 2016 23:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:11:39 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

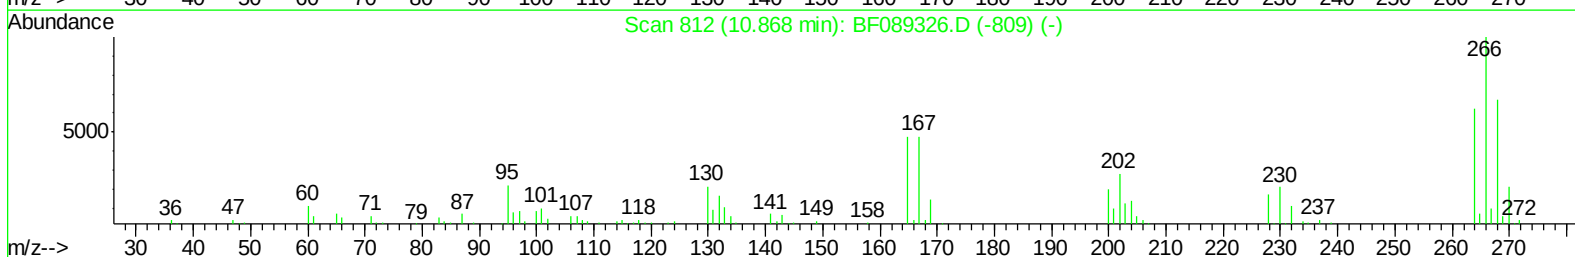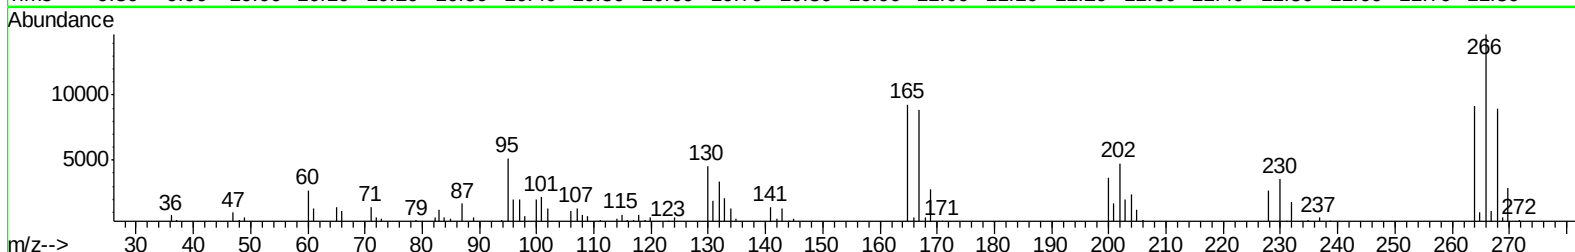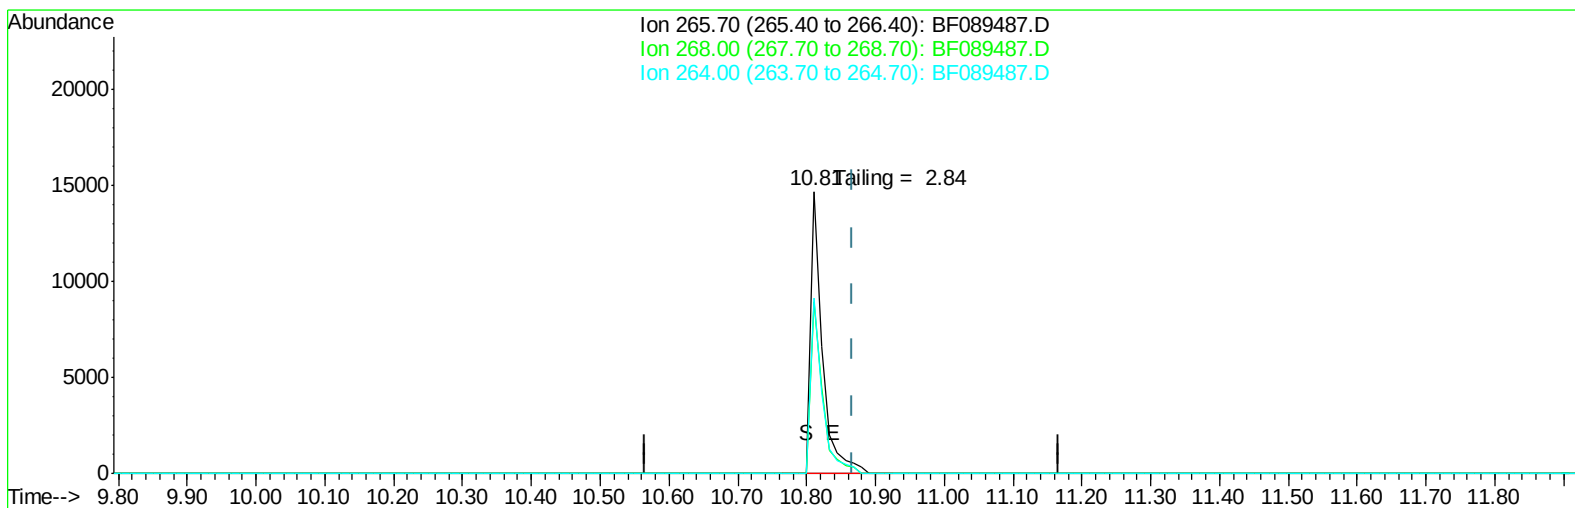

TIC: BF089487.D

(69) Pentachlorophenol (C)

10.810min (-0.057) 0.00ng

response 17693

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	60.87
264.00	62.70	62.41
0.00	0.00	0.00