

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073016\
 Data File : BF089440.D
 Acq On : 30 Jul 2016 6:40
 Operator : UM/SJ
 Sample : H4206-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LOCATION-61A

Quant Time: Aug 01 01:10:16 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 16:02:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.51	152	39934	20.00	ng	-0.03
21) Naphthalene-d8	7.80	136	158176	20.00	ng	-0.02
38) Acenaphthene-d10	9.54	164	73599	20.00	ng	-0.03
63) Phenanthrene-d10	11.02	188	113007	20.00	ng	-0.03
75) Chrysene-d12	13.63	240	78770	20.00	ng	-0.03
86) Perylene-d12	14.96	264	83871	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.08	112	350872	140.29	ng	-0.02
7) Phenol-d6	6.17	99	462934	140.06	ng	-0.03
23) Nitrobenzene-d5	7.08	82	281551	105.06	ng	-0.03
41) 2,4,6-Tribromophenol	10.33	330	74670	122.50	ng	-0.03
44) 2-Fluorobiphenyl	8.88	172	487765	97.26	ng	-0.03
78) Terphenyl-d14	12.59	244	297401	88.37	ng	-0.03
Target Compounds						
10) Phenol	6.19	94	8524	2.34	ng	# 82
49) Dimethylphthalate	9.28	163	149722	26.73	ng	99
83) Bis(2-ethylhexyl)phthalate	13.63	149	20583	5.25	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073016\
Data File : BF089440.D
Acq On : 30 Jul 2016 6:40
Operator : UM/SJ
Sample : H4206-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LOCATION-61A

Quant Time: Aug 01 01:10:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

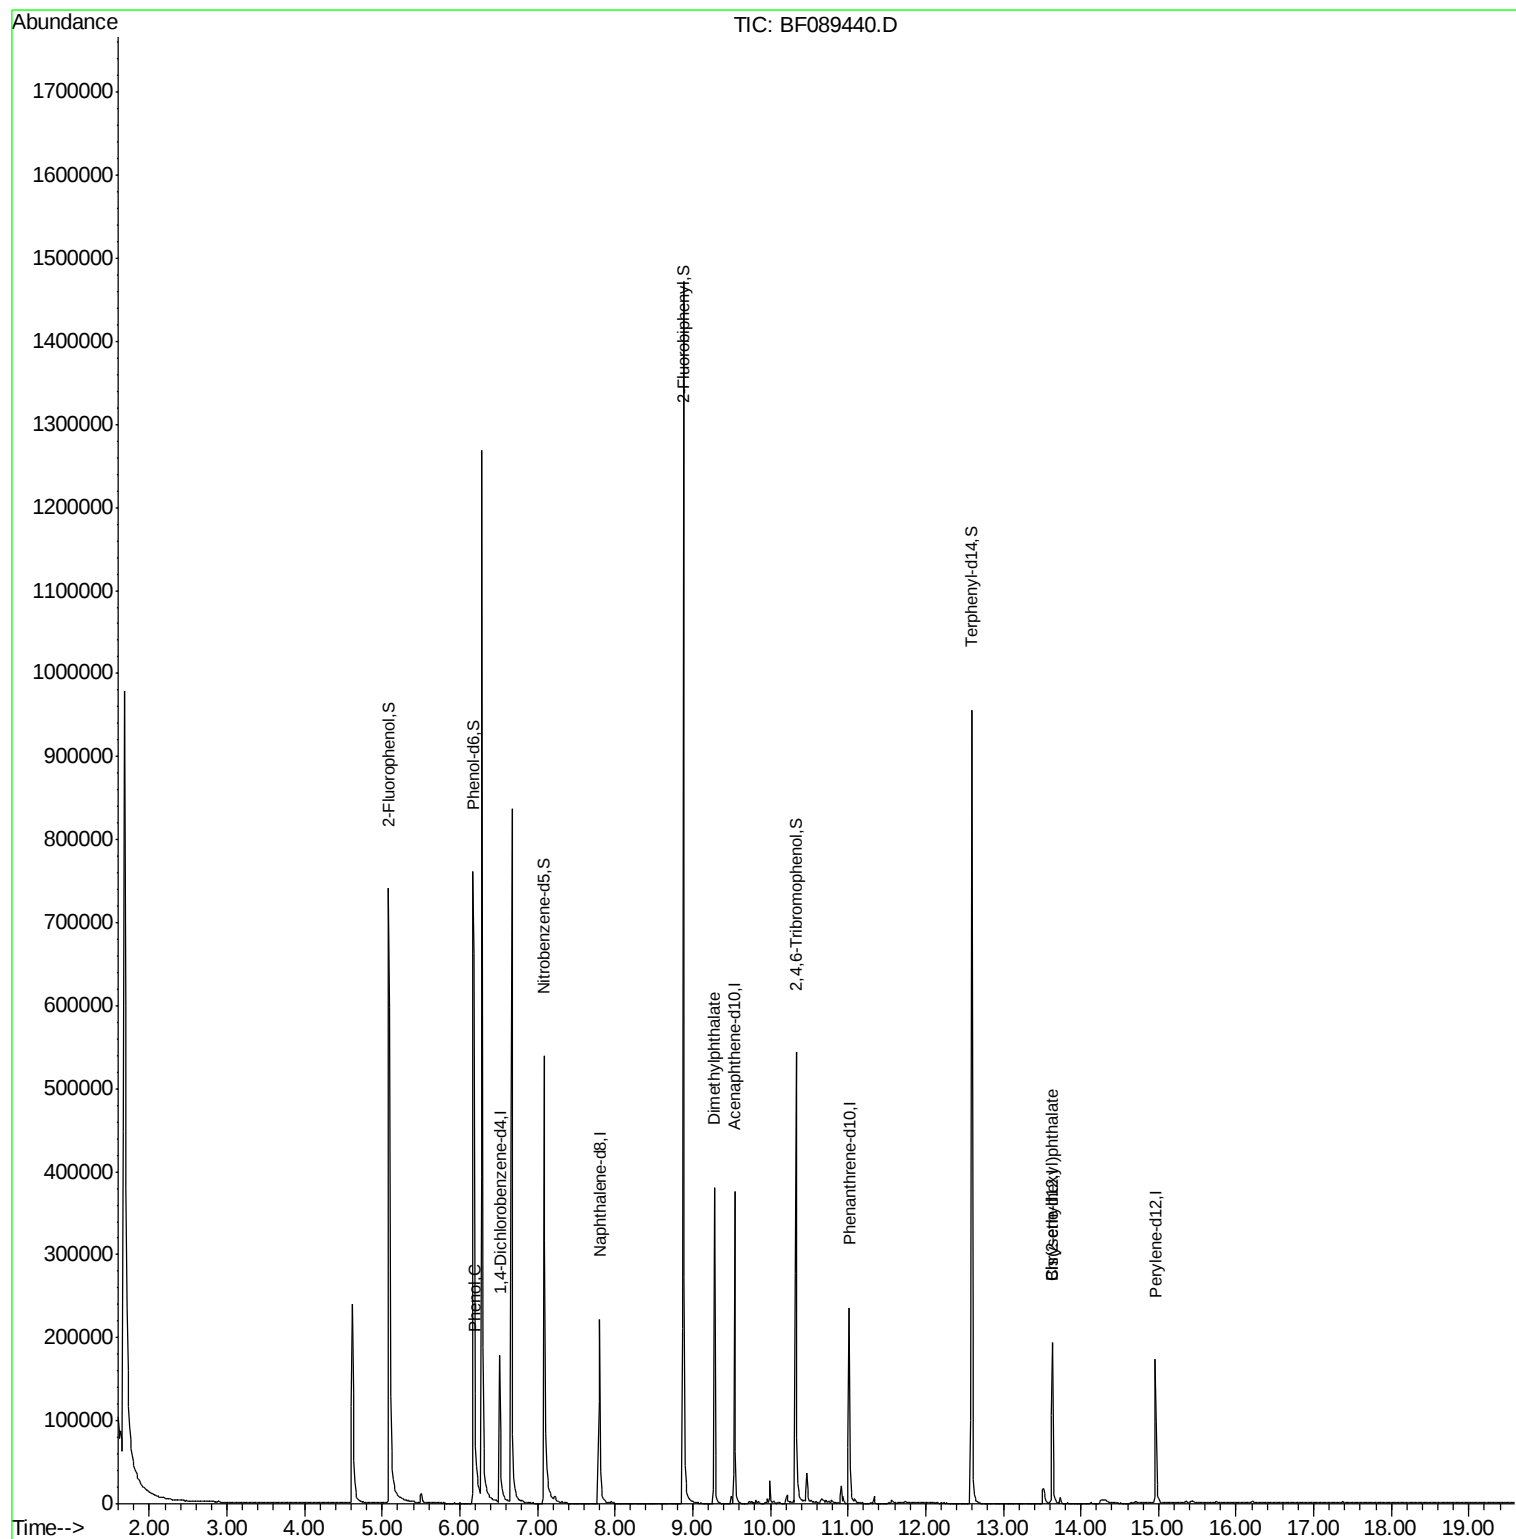



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.51 min Scan# 431

Delta R.T. -0.03 min

Lab File: BF089440.D

Acq: 30 Jul 2016 6:40

Instrument :

BNA_F

ClientSampleId :

LOCATION-61A


Tgt Ion:152 Resp: 39934

Ion Ratio Lower Upper

152 100

150 160.7 129.5 194.3



115 72.0 51.4 77.2

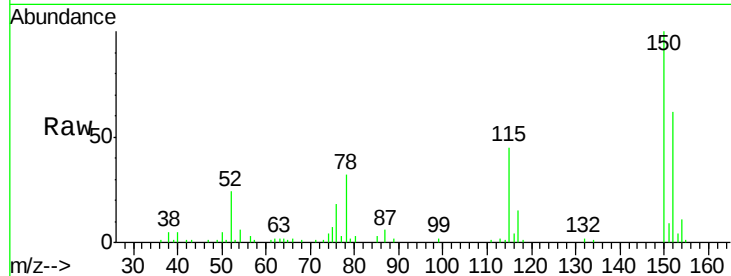

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

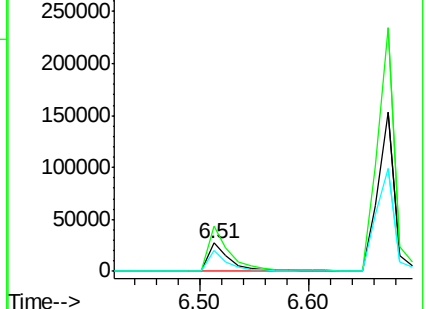

#5

2-Fluorophenol

Concen: 140.29 ng

RT: 5.08 min Scan# 306

Delta R.T. -0.02 min

Lab File: BF089440.D

Acq: 30 Jul 2016 6:40


Tgt Ion:112 Resp: 350872

Ion Ratio Lower Upper

112 100

64 65.8 55.0 82.6



63 35.4 29.4 44.2

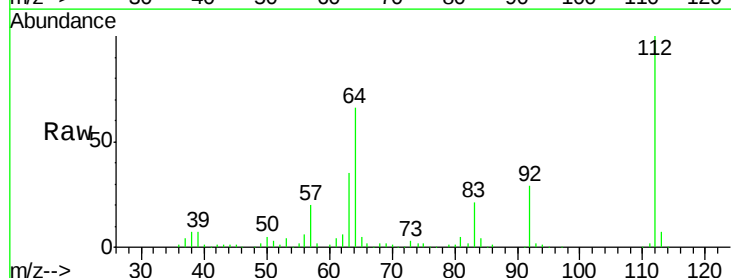

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

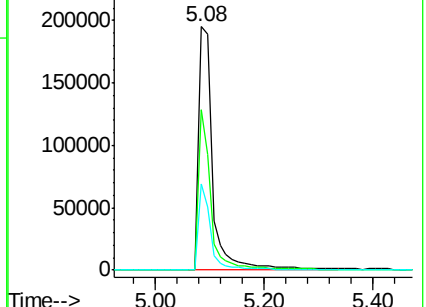



#7

Phenol-d6

Concen: 140.06 ng

RT: 6.17 min Scan# 401

Delta R.T. -0.03 min

Lab File: BF089440.D

Acq: 30 Jul 2016 6:40

Instrument :

BNA_F

ClientSampleId :

LOCATION-61A


Tgt Ion: 99 Resp: 462934

Ion Ratio Lower Upper

99 100

42 19.2 13.6 20.4




71 39.2 29.4 44.2

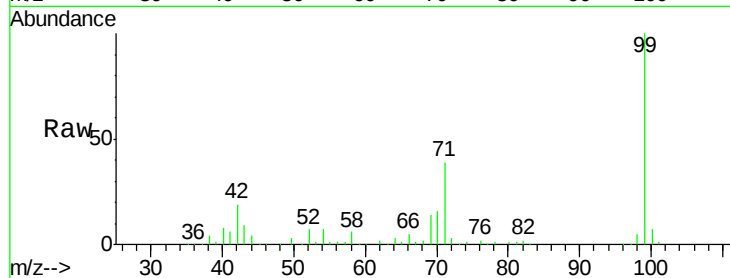

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

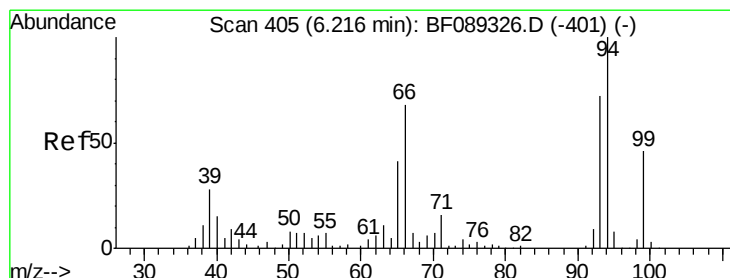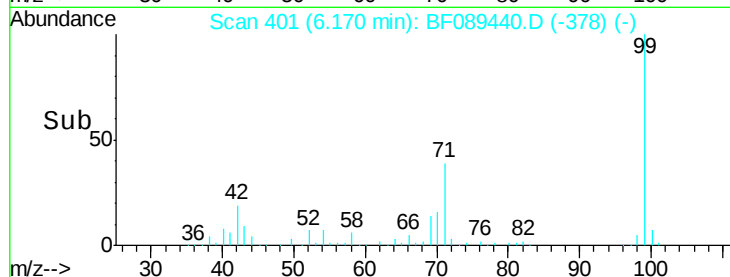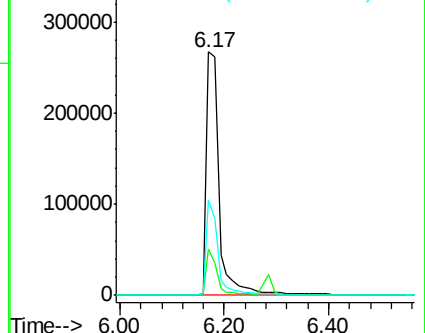

#10

Phenol

Concen: 2.34 ng

RT: 6.19 min Scan# 403

Delta R.T. -0.02 min

Lab File: BF089440.D

Acq: 30 Jul 2016 6:40


Tgt Ion: 94 Resp: 8524

Ion Ratio Lower Upper

94 100

65 36.8 19.1 59.1



66 85.3 44.4 84.4#

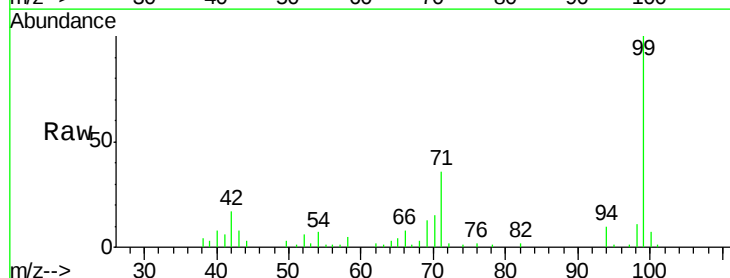


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

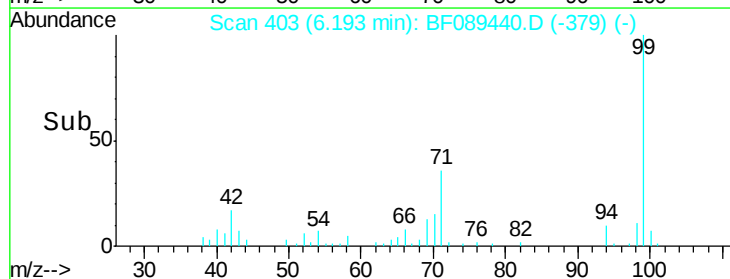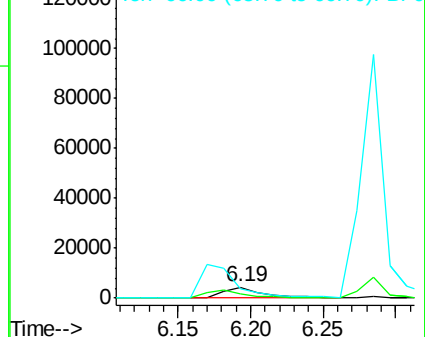


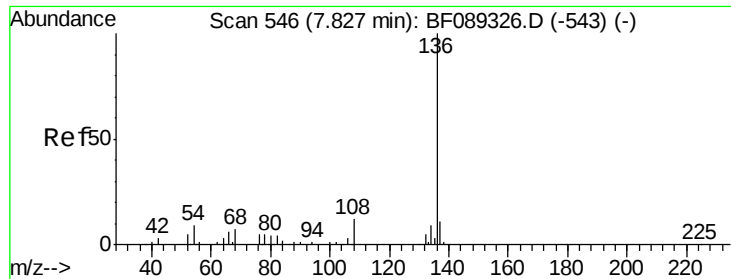




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.80 min Scan# 544
Delta R.T. -0.02 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Instrument :
BNA_F
ClientSampleId :
LOCATION-61A

Tgt Ion:	136	Resp:	158176
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	13.0
54	6.1	7.0	10.4#
68	4.6	4.9	7.3#

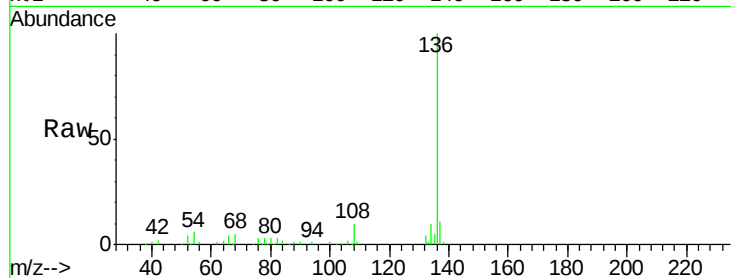


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

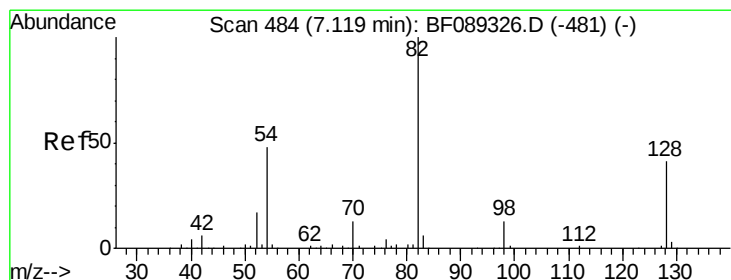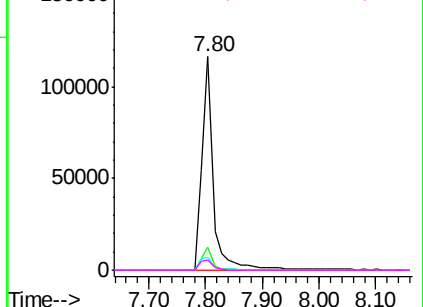




#23
Nitrobenzene-d5
Concen: 105.06 ng
RT: 7.08 min Scan# 481
Delta R.T. -0.03 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Tgt Ion:	82	Resp:	281551
Ion	Ratio	Lower	Upper
82	100		
128	37.3	32.5	48.7
54	49.6	38.8	58.2

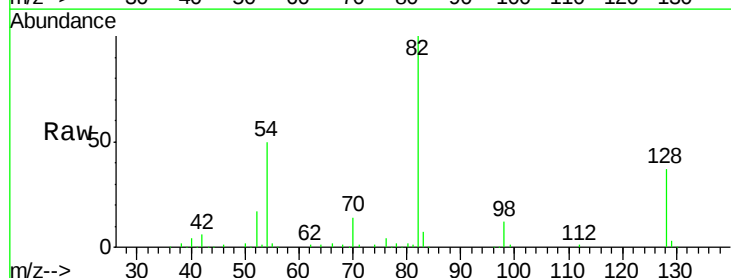

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

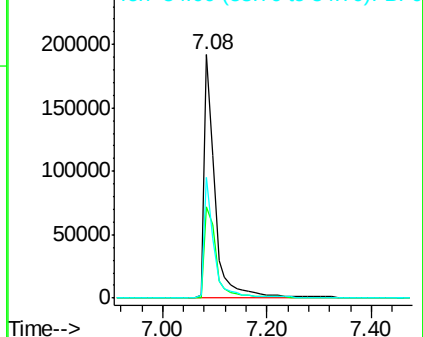







#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.54 min Scan# 696
 Delta R.T. -0.03 min
 Lab File: BF089440.D
 Acq: 30 Jul 2016 6:40

Instrument :
 BNA_F
 ClientSampleId :
 LOCATION-61A

Tgt Ion:164 Resp: 73599
 Ion Ratio Lower Upper
 164 100
 162 107.7 83.7 125.5
 160 45.4 37.8 56.6

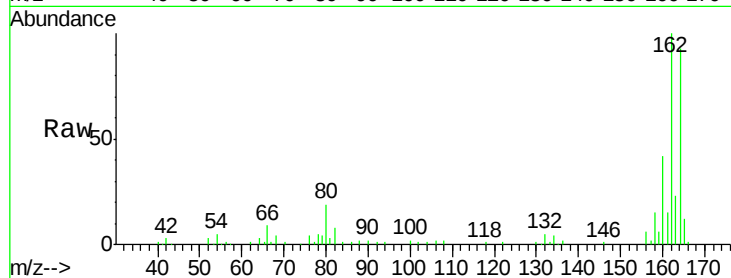


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

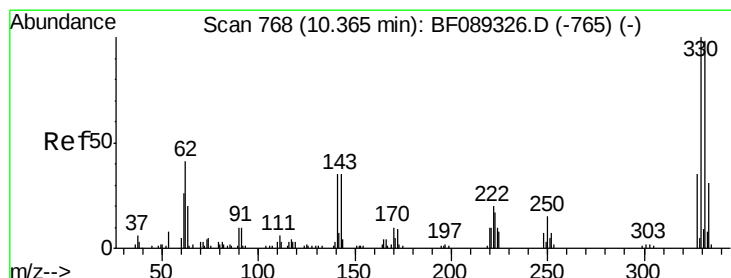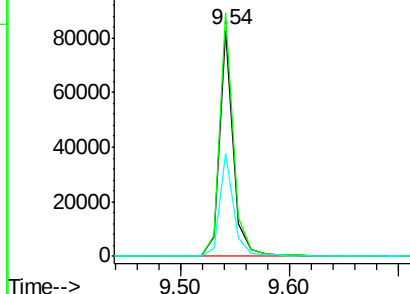




#41
 2,4,6-Tribromophenol
 Concen: 122.50 ng
 RT: 10.33 min Scan# 765
 Delta R.T. -0.03 min
 Lab File: BF089440.D
 Acq: 30 Jul 2016 6:40

Tgt Ion:330 Resp: 74670
 Ion Ratio Lower Upper
 330 100
 332 94.7 76.8 115.2
 141 45.6 37.3 55.9

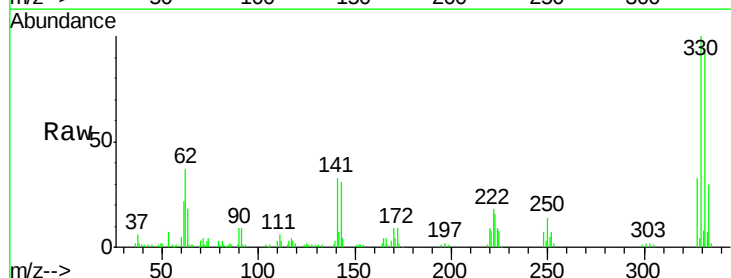

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



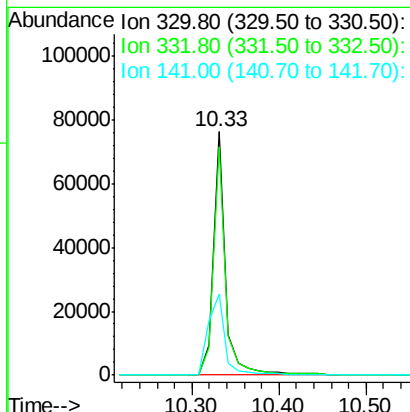



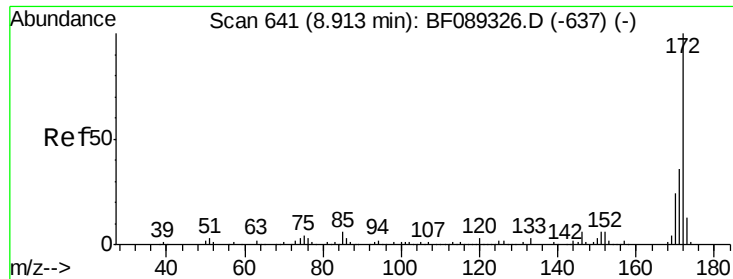

#44
2-Fluorobiphenyl
Concen: 97.26 ng
RT: 8.88 min Scan# 638
Delta R.T. -0.03 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40




Instrument :
BNA_F
ClientSampleId :
LOCATION-61A


Tgt Ion:172 Resp: 487765
Ion Ratio Lower Upper
172 100
171 35.8 29.2 43.8
170 23.8 19.2 28.8

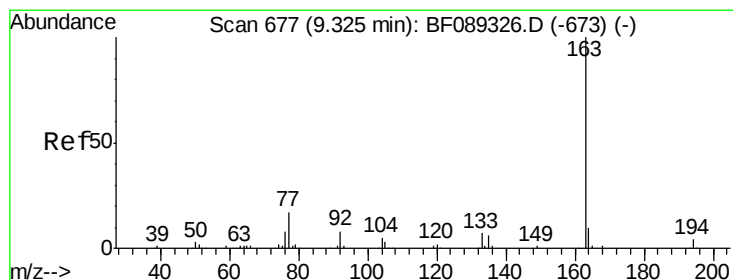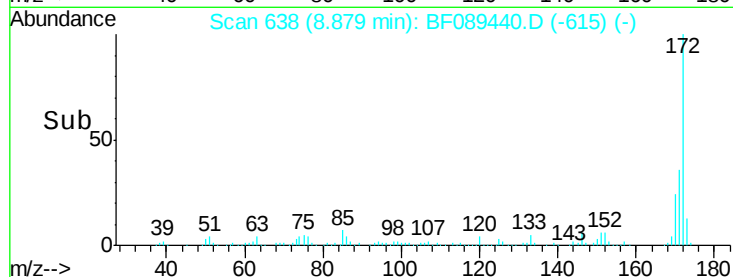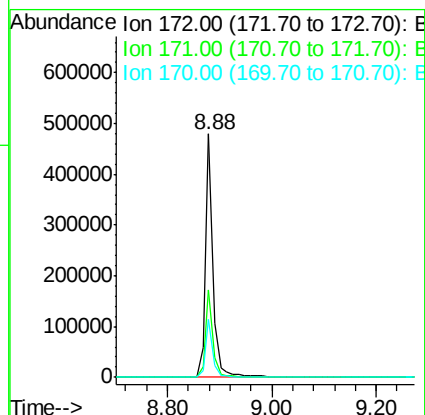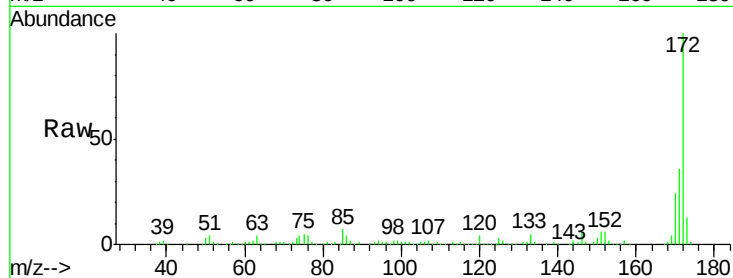

#49
Dimethylphthalate
Concen: 26.73 ng
RT: 9.28 min Scan# 673
Delta R.T. -0.05 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Tgt Ion:163 Resp: 149722
Ion Ratio Lower Upper
163 100
194 3.0 2.8 4.2
164 10.2 7.8 11.8

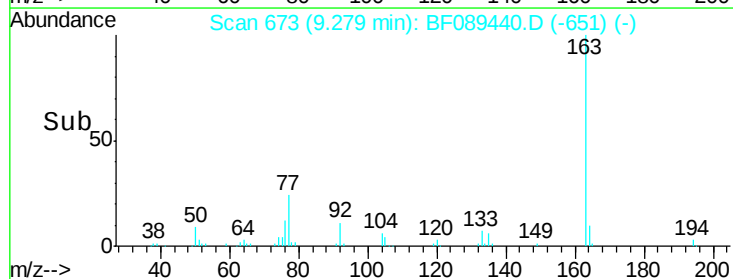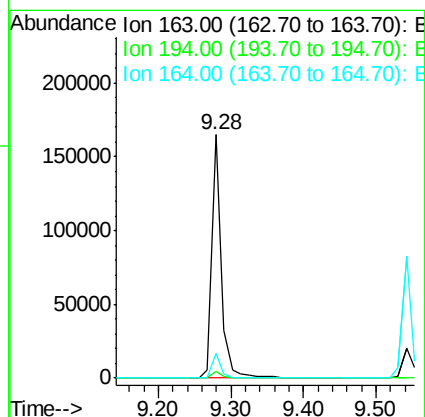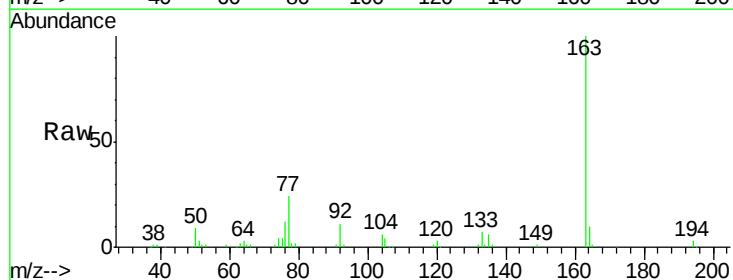


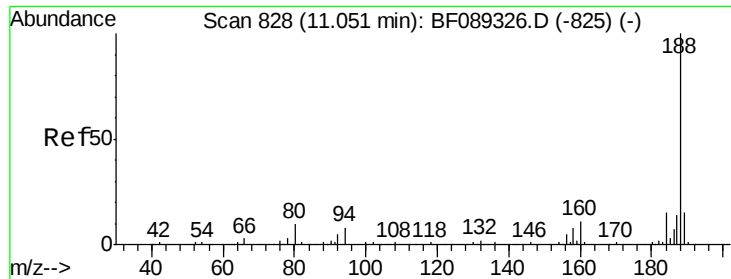




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.02 min Scan# 825
Delta R.T. -0.03 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Instrument :
BNA_F
ClientSampleId :
LOCATION-61A

Tgt Ion:188 Resp: 113007
Ion Ratio Lower Upper
188 100
94 8.0 6.5 9.7
80 8.9 7.2 10.8

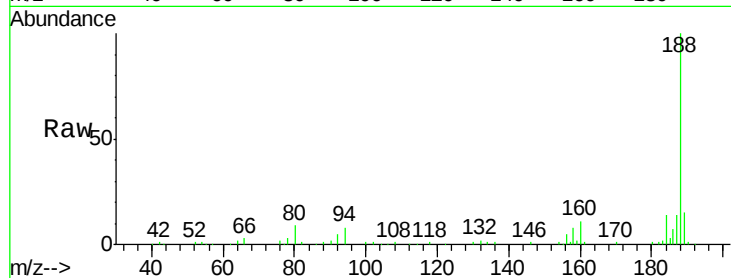


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

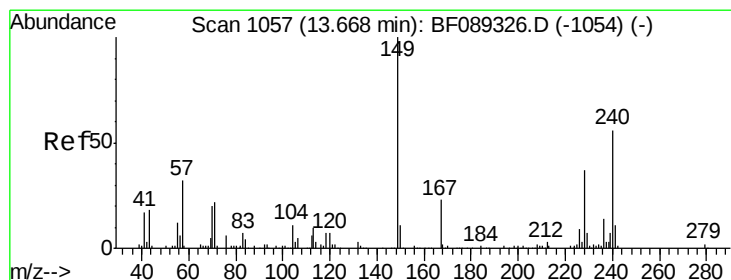
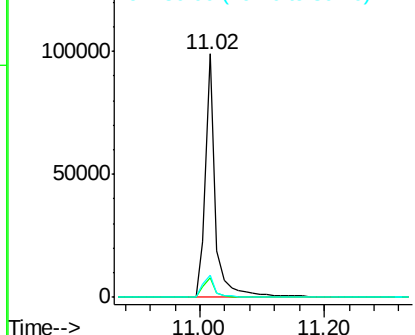



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.63 min Scan# 1054
Delta R.T. -0.03 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Tgt Ion:240 Resp: 78770
Ion Ratio Lower Upper
240 100
120 10.3 9.1 13.7
236 24.9 20.6 30.8

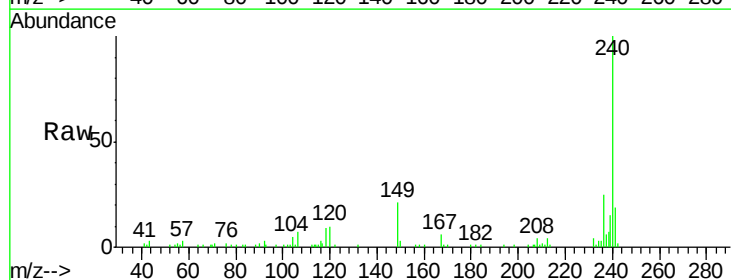

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




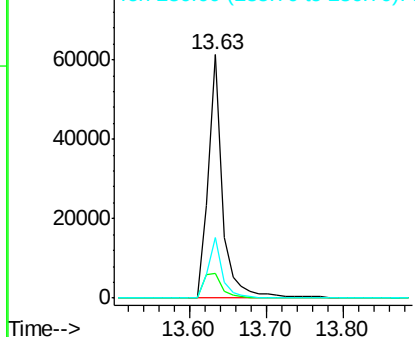


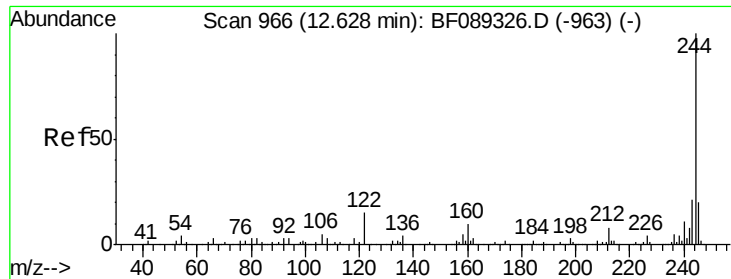

#78
 Terphenyl-d14
 Concen: 88.37 ng
 RT: 12.59 min Scan# 963
 Delta R.T. -0.03 min
 Lab File: BF089440.D
 Acq: 30 Jul 2016 6:40




Instrument :
 BNA_F
 ClientSampleId :
 LOCATION-61A


Tgt Ion:244 Resp: 297401
 Ion Ratio Lower Upper
 244 100
 212 8.2 6.5 9.7
 122 14.4 11.4 17.0

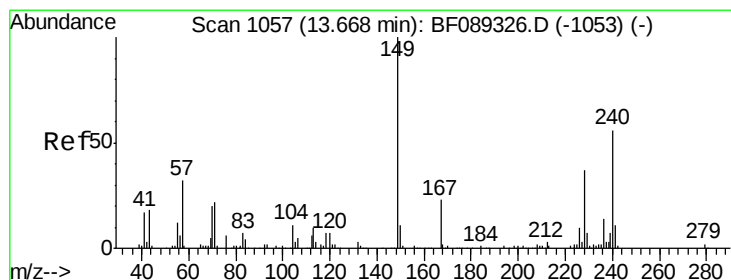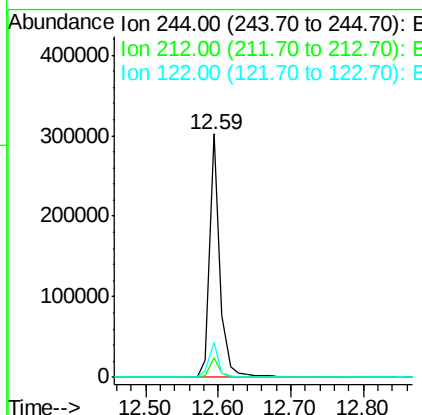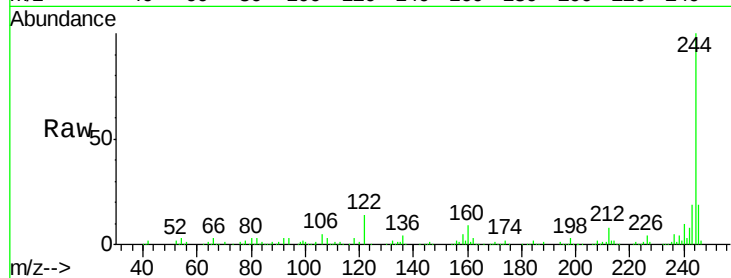

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 5.25 ng
 RT: 13.63 min Scan# 1054
 Delta R.T. -0.03 min
 Lab File: BF089440.D
 Acq: 30 Jul 2016 6:40

Tgt Ion:149 Resp: 20583
 Ion Ratio Lower Upper
 149 100
 167 27.6 18.8 28.2
 279 0.0 1.4 2.0#

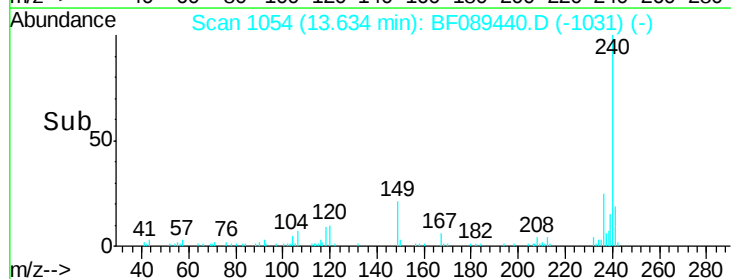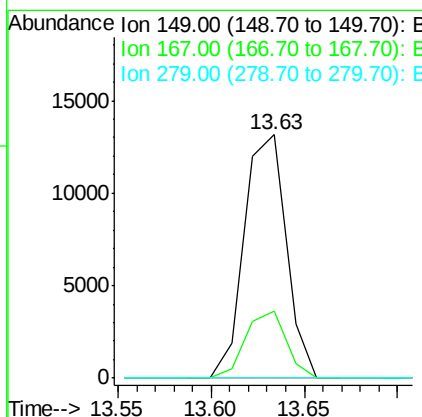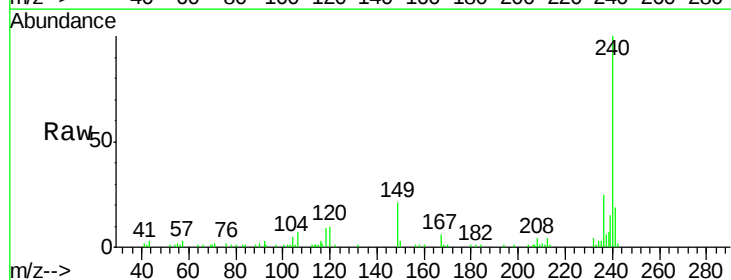

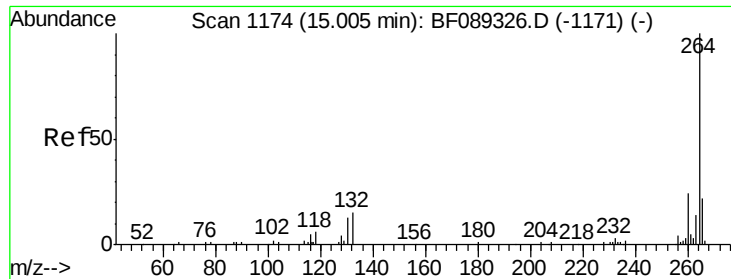

#86
Perylene-d12
Concen: 20.00 ng
RT: 14.96 min Scan# 1170
Delta R.T. -0.05 min
Lab File: BF089440.D
Acq: 30 Jul 2016 6:40

Instrument :
BNA_F
ClientSampleId :
LOCATION-61A

Tgt Ion: 264 Resp: 83871
Ion Ratio Lower Upper
264 100
260 22.9 19.0 28.4
265 21.6 17.5 26.3

