


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073016\
 Data File : BF089438.D
 Acq On : 30 Jul 2016 5:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

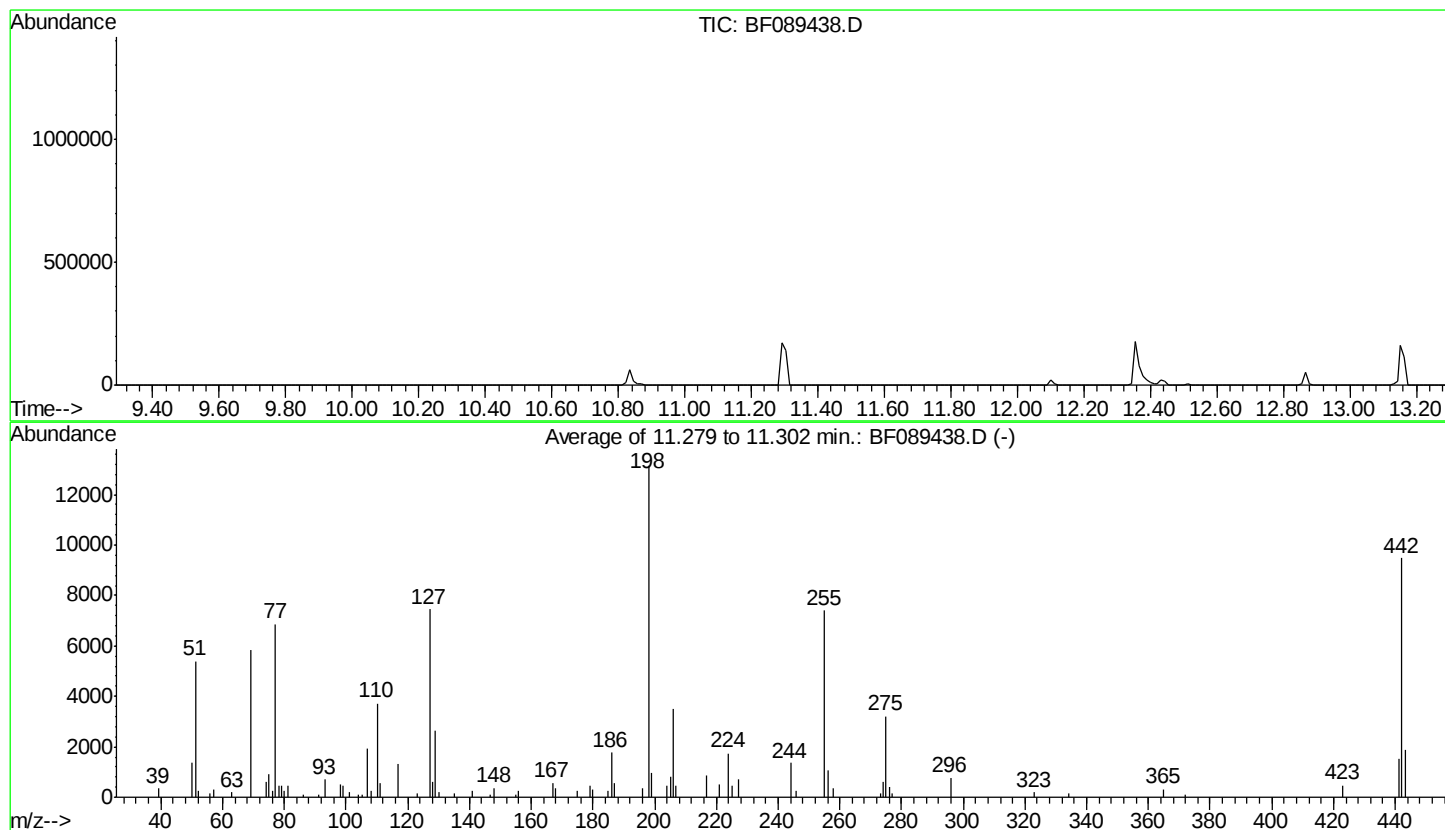

AutoFind: Scans 848, 849, 850; Background Corrected with Scan 846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	5403	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.4	5841	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	7461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13149	PASS
199	198	5	9	7.3	965	PASS
275	198	10	60	24.5	3216	PASS
365	198	1	100	2.4	311	PASS
441	442	0.01	24	15.8	1504	PASS
442	198	50	100	72.2	9491	PASS
443	442	15	24	19.6	1857	PASS