
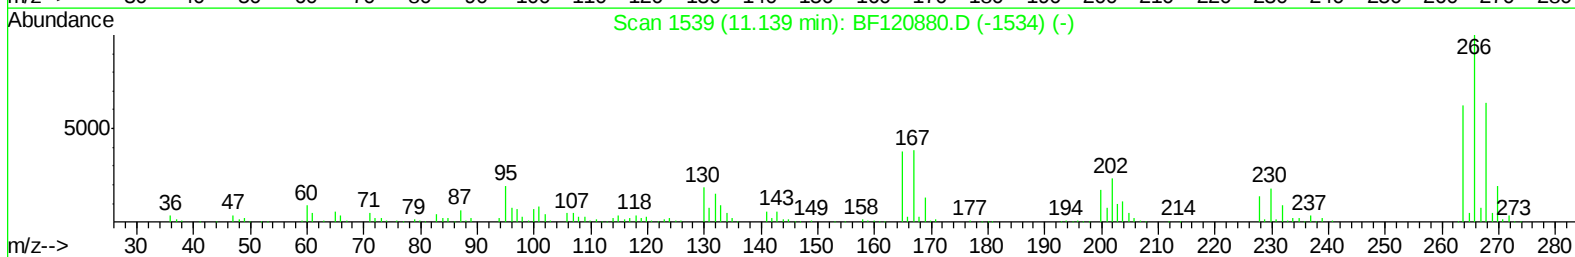
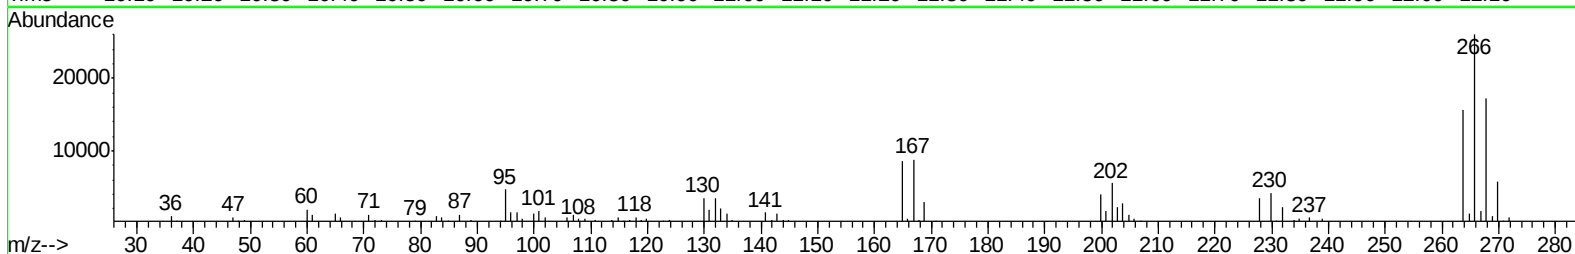


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073020\
Data File : BF121125.D
Acq On : 30 Jul 2020 13:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 07:13:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 14:55:43 2020
Response via : Initial Calibration

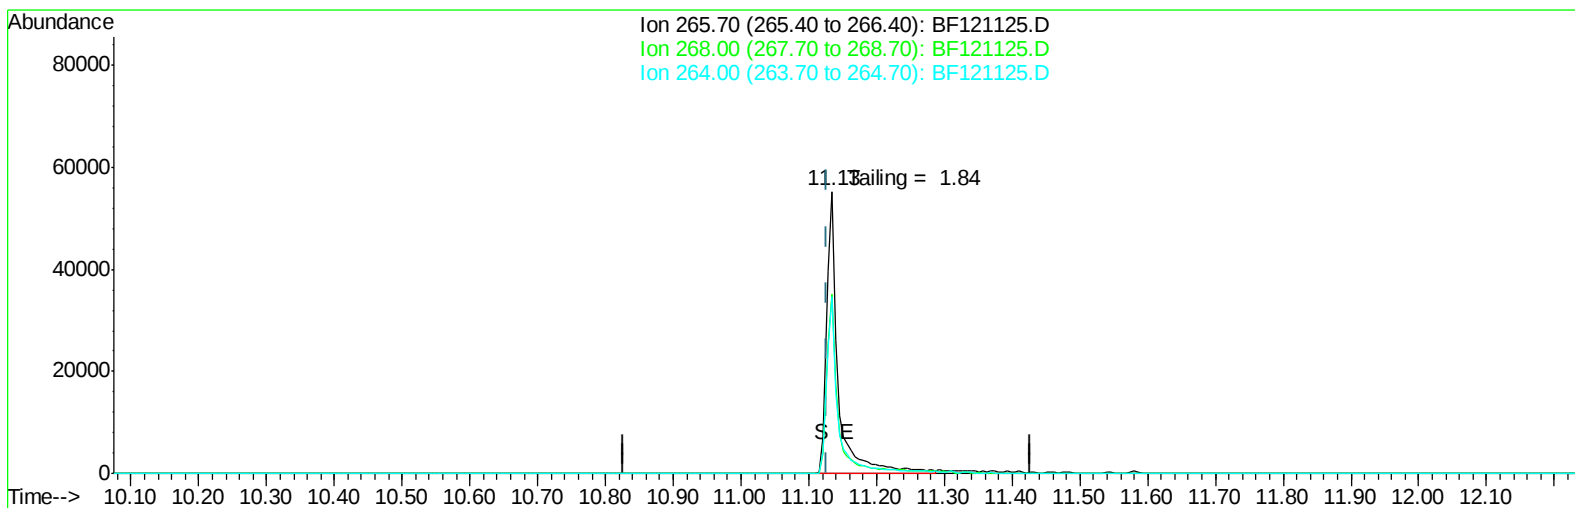

TIC: BF121125.D

(70) Pentachlorophenol (C)




11.133min (+0.006) 22603.72ng

response 63095

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.59
264.00	63.00	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073020\
 Data File : BF121125.D
 Acq On : 30 Jul 2020 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 07:13:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

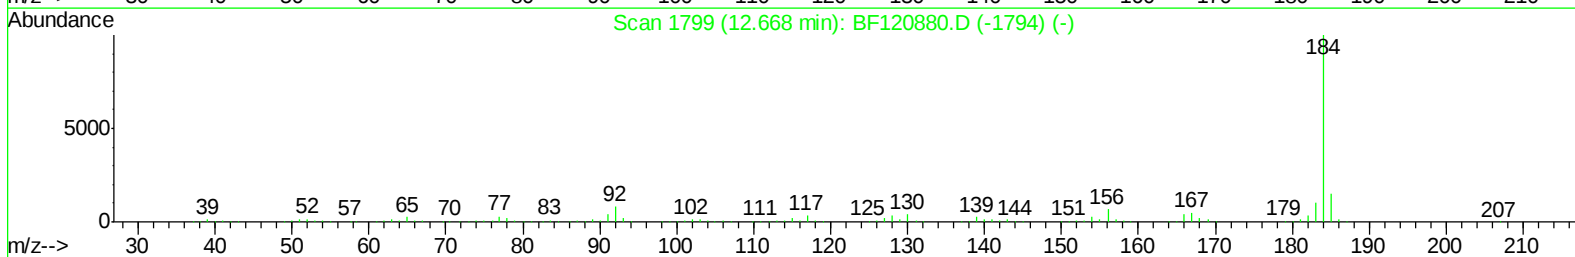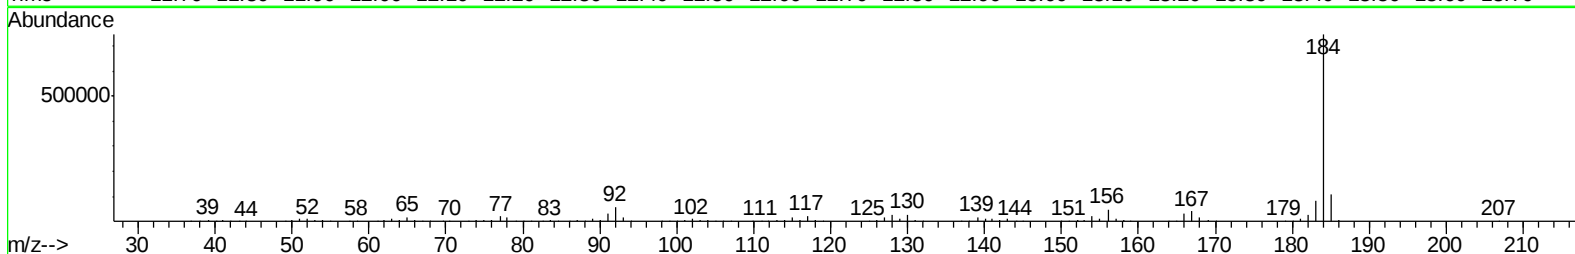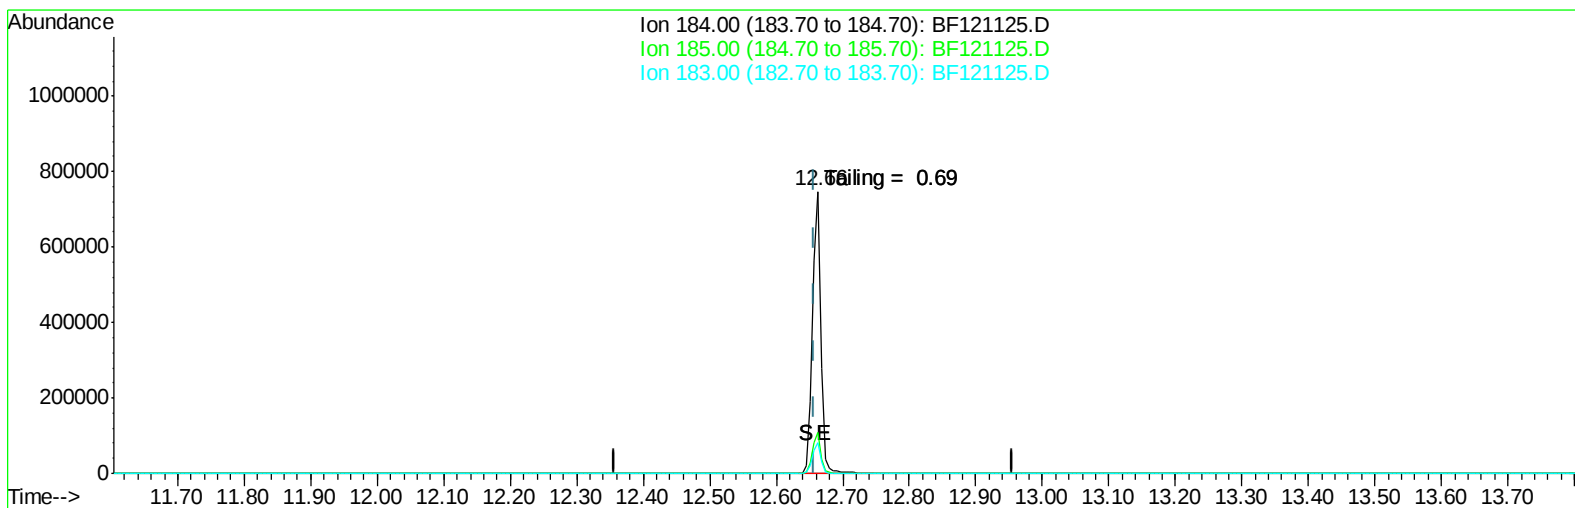

TIC: BF121125.D

(77) Benzidine

12.663min (+0.006) 0.00ng

response 667666

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.48
183.00	11.20	11.08
0.00	0.00	0.00