

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073020\
 Data File : BF121144.D
 Acq On : 30 Jul 2020 23:24
 Operator : JU/CG
 Sample : L3451-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-03-015-A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.793	286	290	299	rVB	19081	28562	2.74%	0.293%
2	5.410	562	565	580	rVB	541373	519604	49.91%	5.330%
3	6.434	736	739	752	rBV	582351	546806	52.52%	5.609%
4	6.798	798	801	805	rBV	869319	715355	68.71%	7.337%
5	7.357	893	896	901	rBV	362480	304959	29.29%	3.128%
6	8.086	1016	1020	1023	rBV	998836	888714	85.36%	9.116%
7	8.145	1027	1030	1032	rVB	13412	13775	1.32%	0.141%
8	8.504	1088	1091	1093	rBV	18496	16540	1.59%	0.170%
9	8.675	1118	1120	1124	rBV2	28046	21697	2.08%	0.223%
10	9.110	1191	1194	1199	rBV	20264	20870	2.00%	0.214%
11	9.157	1199	1202	1208	rBV	806296	662562	63.64%	6.796%
12	9.239	1213	1216	1219	rBV	41536	40930	3.93%	0.420%
13	9.551	1266	1269	1273	rBV2	79465	91393	8.78%	0.937%
14	9.704	1292	1295	1300	rBV	26528	26206	2.52%	0.269%
15	9.774	1304	1307	1311	rVB	36316	33249	3.19%	0.341%
16	9.839	1315	1318	1322	rBV	1145393	968613	93.04%	9.935%
17	9.998	1340	1345	1348	rBV6	7889	13682	1.31%	0.140%
18	10.045	1348	1353	1358	rVV4	12461	22767	2.19%	0.234%
19	10.086	1358	1360	1366	rVV4	10738	16170	1.55%	0.166%
20	10.269	1389	1391	1394	rVB	37727	32278	3.10%	0.331%
21	10.386	1408	1411	1418	rBV4	8448	13762	1.32%	0.141%
22	10.492	1425	1429	1434	rVB2	22134	28779	2.76%	0.295%
23	10.627	1449	1452	1460	rVB	319322	306025	29.39%	3.139%
24	10.745	1468	1472	1478	rBV3	53336	82928	7.97%	0.851%
25	11.192	1543	1548	1551	rBV2	38931	41239	3.96%	0.423%
26	11.221	1551	1553	1559	rVB	28118	31565	3.03%	0.324%
27	11.327	1567	1571	1574	rBV	1097926	950796	91.33%	9.752%
28	11.404	1582	1584	1587	rVB	35430	27483	2.64%	0.282%
29	11.621	1618	1621	1625	rVB	39139	31523	3.03%	0.323%
30	11.668	1625	1629	1635	rBV6	9625	18094	1.74%	0.186%
31	11.786	1645	1649	1652	rBV5	9516	16970	1.63%	0.174%
32	11.833	1654	1657	1659	rVV2	20431	25663	2.47%	0.263%
33	11.863	1659	1662	1664	rVB	22146	23661	2.27%	0.243%
34	11.939	1673	1675	1678	rBV2	33012	31990	3.07%	0.328%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073020\
Data File : BF121144.D
Acq On : 30 Jul 2020 23:24
Operator : JU/CG
Sample : L3451-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-03-015-A

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.027	1687	1690	1693	rBV	35777	30384	2.92%	0.312%
36	12.127	1704	1707	1709	rBV3	13461	14885	1.43%	0.153%
37	12.304	1734	1737	1740	rBV2	35357	35949	3.45%	0.369%
38	12.380	1747	1750	1752	rBV	27547	25979	2.50%	0.266%
39	12.415	1753	1756	1761	rVB2	44045	56141	5.39%	0.576%
40	12.539	1774	1777	1782	rBV	163430	159616	15.33%	1.637%
41	12.768	1811	1816	1819	rBV	160712	191761	18.42%	1.967%
42	12.910	1837	1840	1844	rBV	696065	633009	60.80%	6.493%
43	13.145	1878	1880	1882	rBV2	33093	31017	2.98%	0.318%
44	13.974	2016	2021	2023	rBV	996646	1041086	100.00%	10.678%
45	15.433	2265	2269	2280	rVB	618854	914425	87.83%	9.379%


Sum of corrected areas: 9749462

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073020\
Data File : BF121144.D
Acq On : 30 Jul 2020 23:24
Operator : JU/CG
Sample : L3451-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-03-015-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

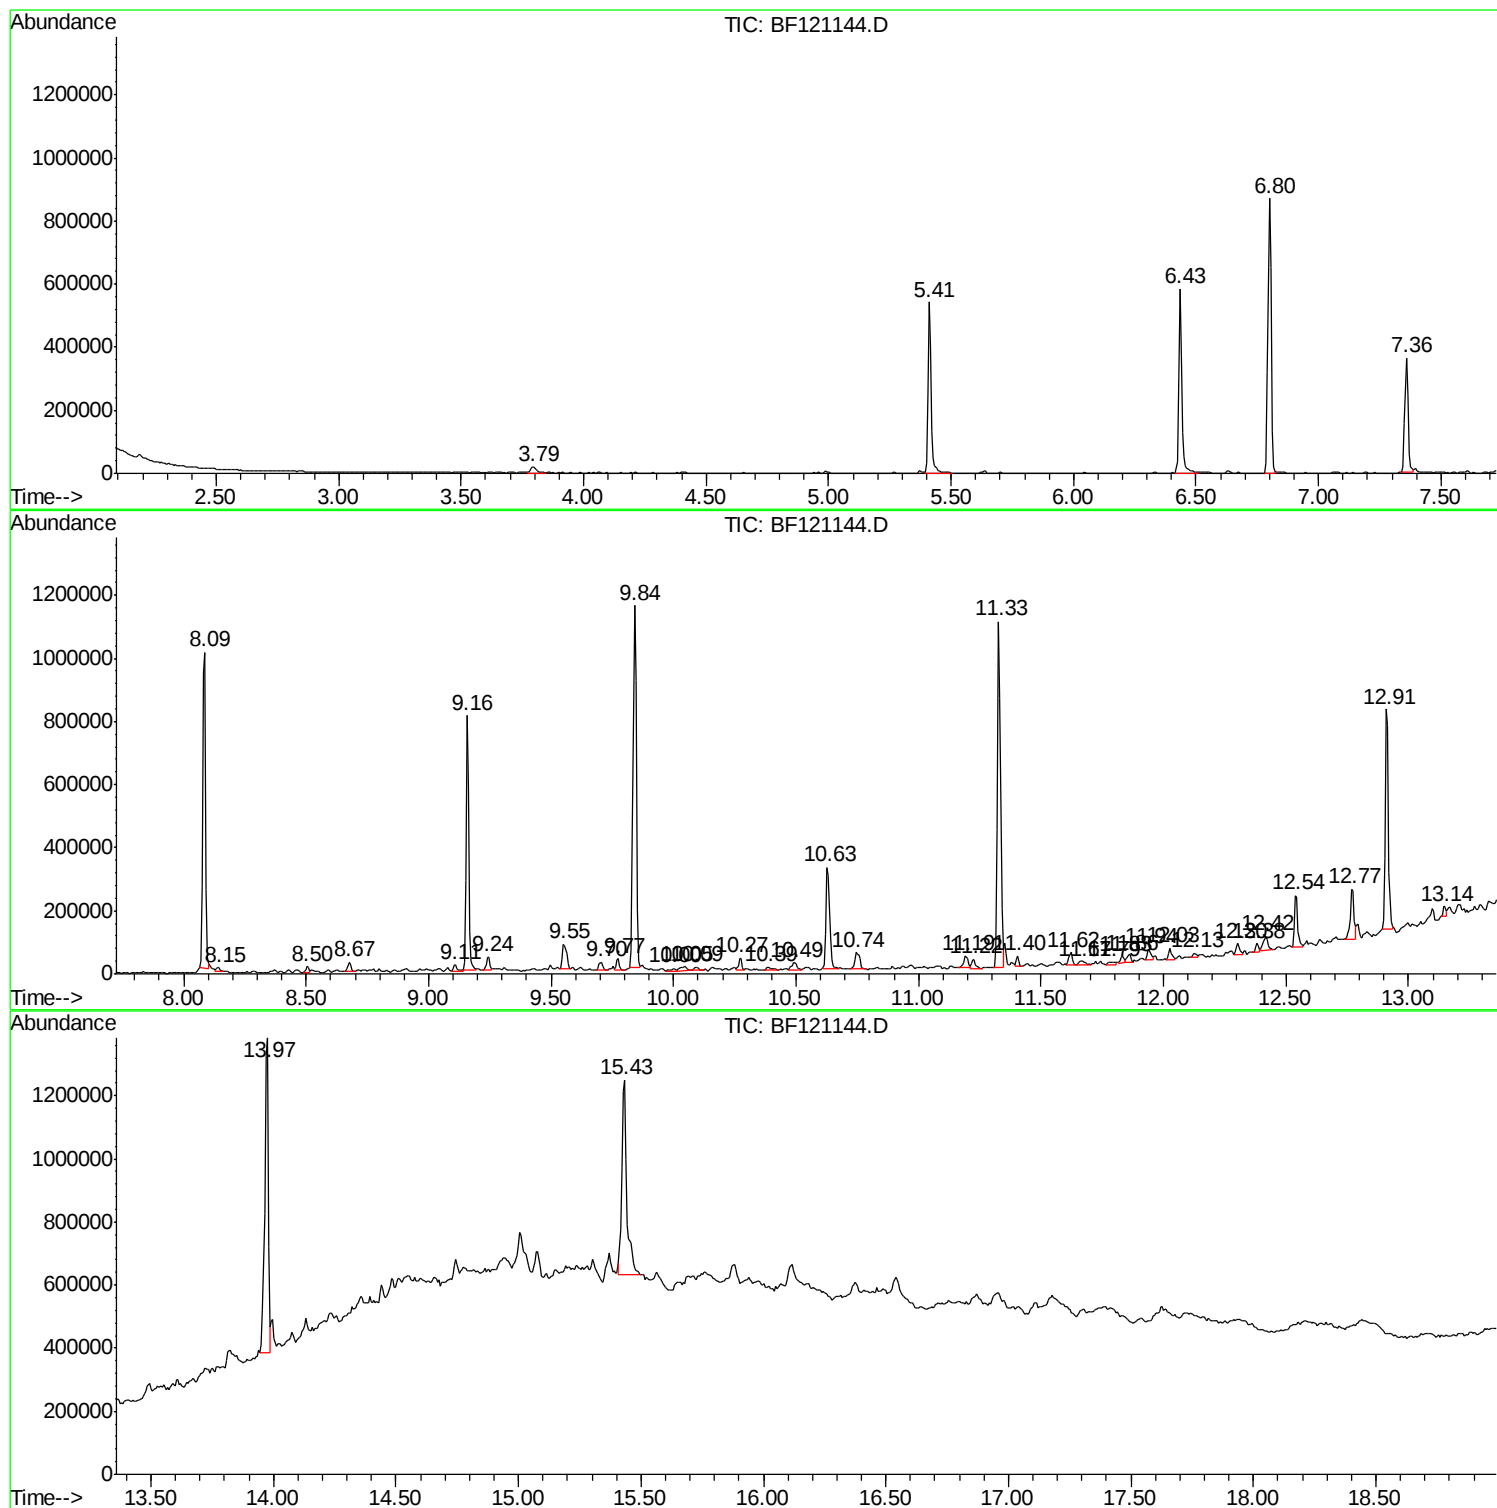

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073020\
Data File : BF121144.D
Acq On : 30 Jul 2020 23:24
Operator : JU/CG
Sample : L3451-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-03-015-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073020\
Data File : BF121144.D
Acq On : 30 Jul 2020 23:24
Operator : JU/CG
Sample : L3451-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-03-015-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc