

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073021\
 Data File : BF124873.D
 Acq On : 30 Jul 2021 13:13
 Operator : JU/CG
 Sample : PB138063BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138063BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	576	581	584	rBB	225280	230856	63.86%	12.639%
2	6.504	745	751	753	rBV	202872	234577	64.89%	12.842%
3	6.869	810	813	816	rBB	58211	43112	11.93%	2.360%
4	7.434	904	909	912	rBV	133950	156891	43.40%	8.589%
5	8.151	1027	1031	1034	rBV	61756	57338	15.86%	3.139%
6	9.228	1208	1214	1217	rBV	284695	309718	85.68%	16.956%
7	9.910	1325	1330	1333	rBV	80666	71547	19.79%	3.917%
8	10.704	1460	1465	1468	rBV	197531	190137	52.60%	10.409%
9	11.398	1579	1583	1586	rBV	91164	74074	20.49%	4.055%
10	12.986	1848	1853	1856	rBV	355804	361500	100.00%	19.791%
11	14.039	2028	2032	2038	rBB	57642	57391	15.88%	3.142%
12	15.515	2278	2283	2291	rBV	25351	39438	10.91%	2.159%




Sum of corrected areas: 1826579

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073021\
Data File : BF124873.D
Acq On : 30 Jul 2021 13:13
Operator : JU/CG
Sample : PB138063BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138063BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

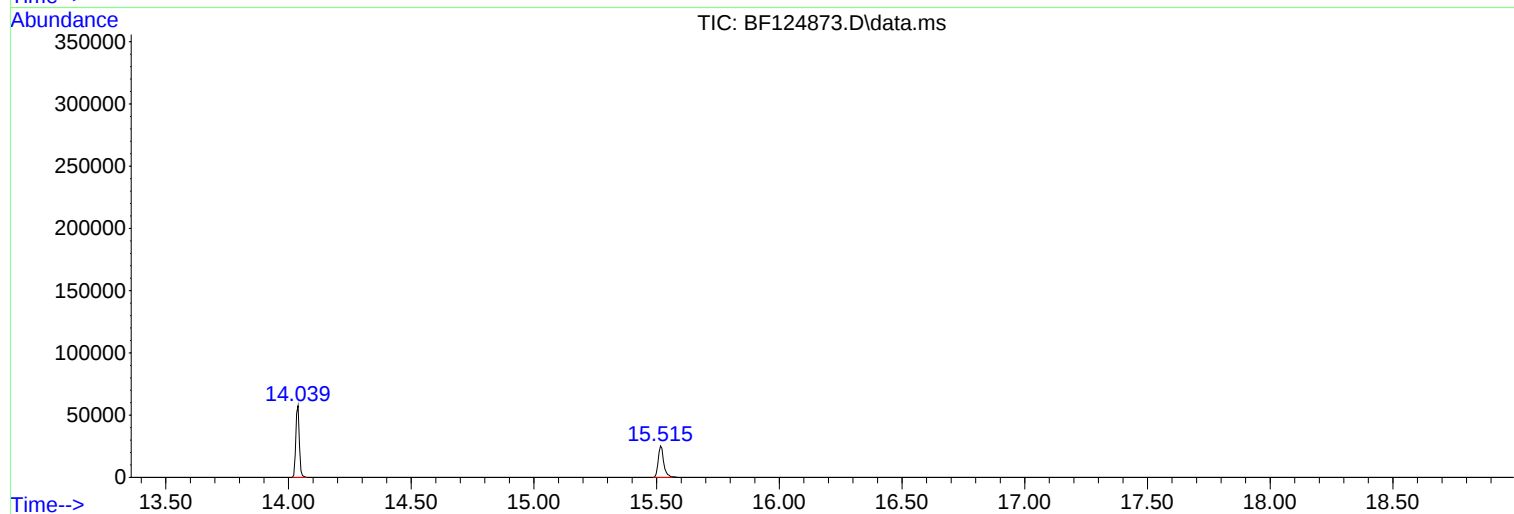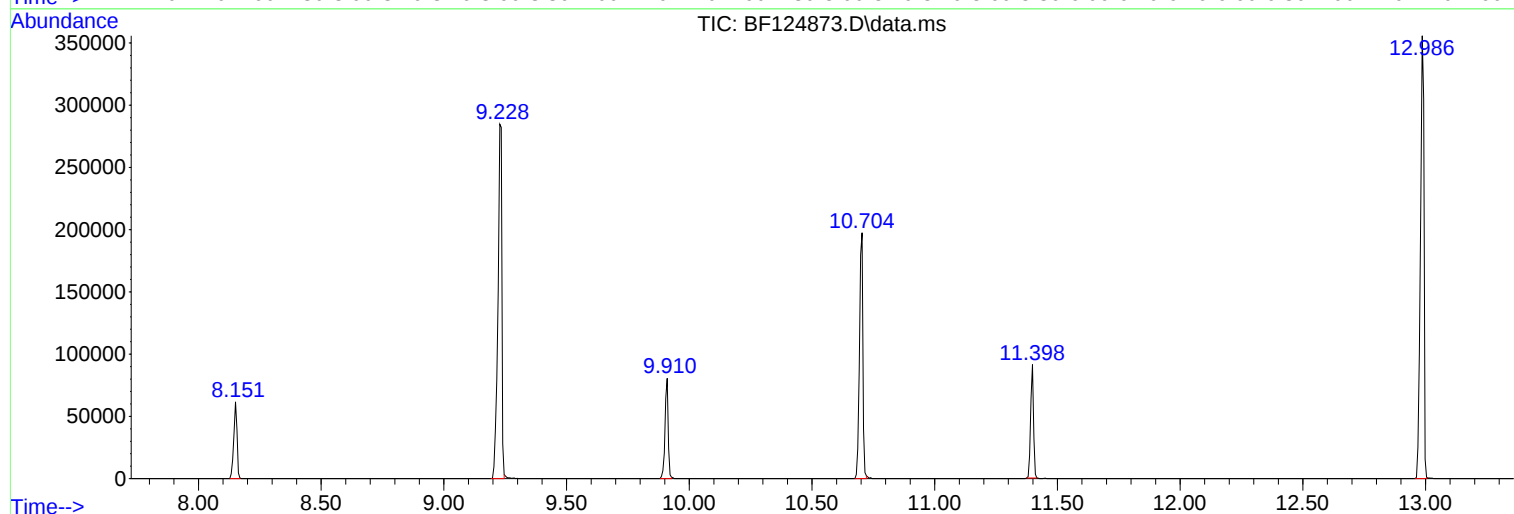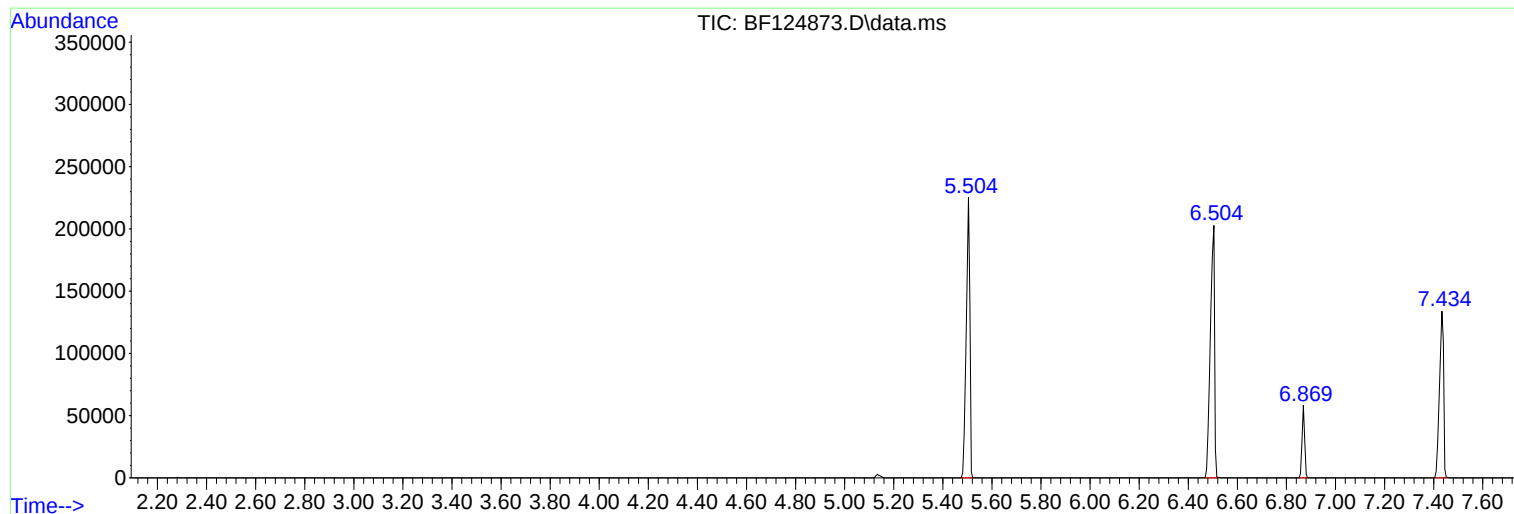

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073021\
Data File : BF124873.D
Acq On : 30 Jul 2021 13:13
Operator : JU/CG
Sample : PB138063BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138063BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073021\
Data File : BF124873.D
Acq On : 30 Jul 2021 13:13
Operator : JU/CG
Sample : PB138063BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138063BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------