
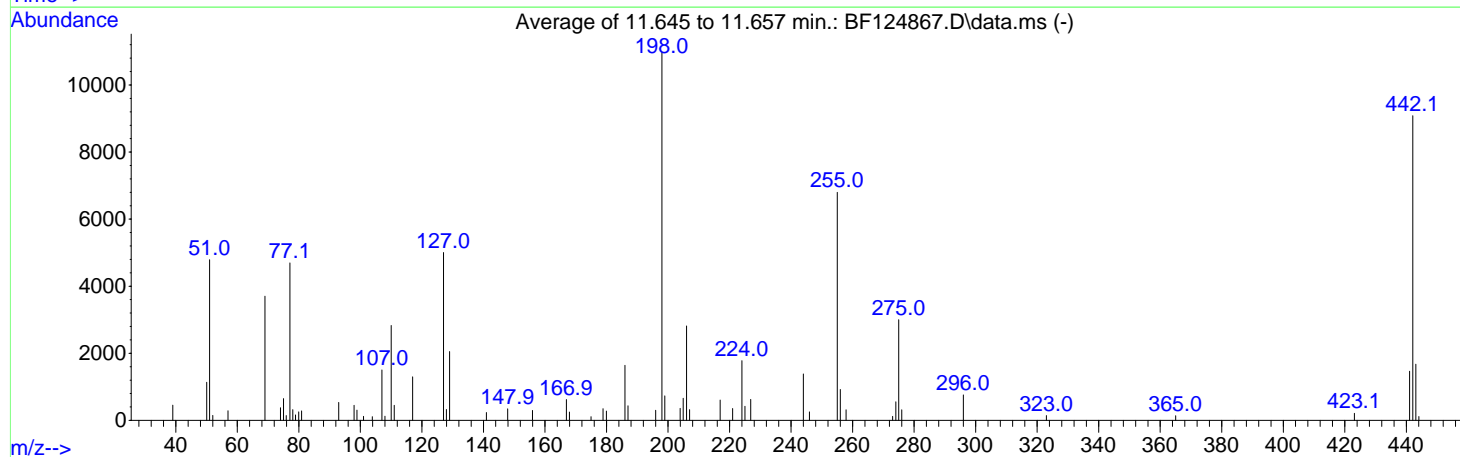


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073021\  
 Data File : BF124867.D  
 Acq On : 30 Jul 2021 8:40  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF072221.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 02 11:15:51 2021

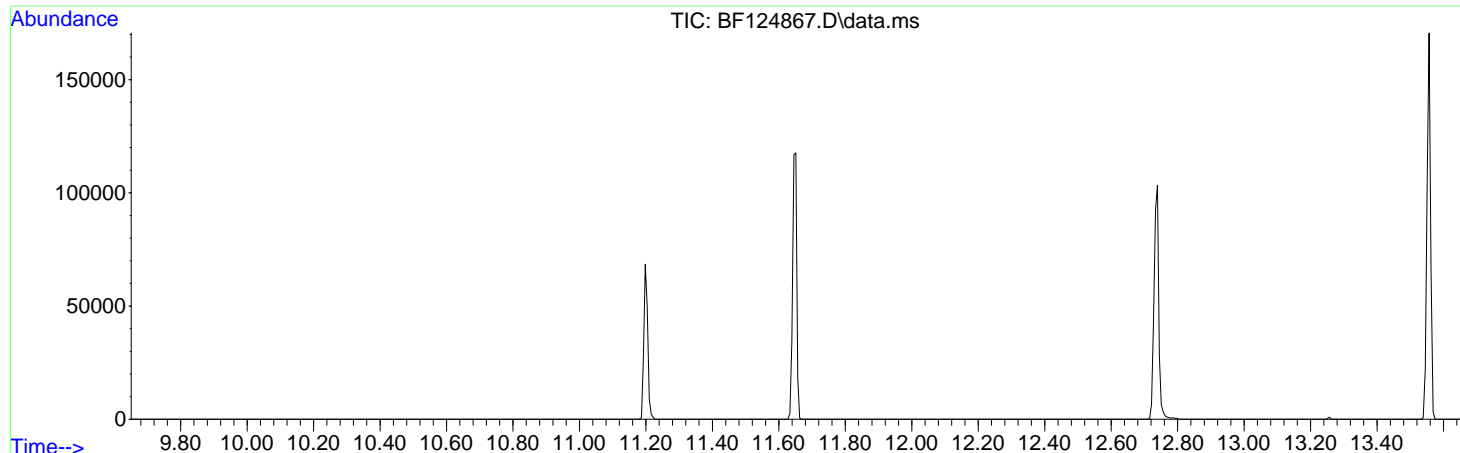




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	4789	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	3701	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	5004	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10969	PASS
199	198	5	9	6.7	732	PASS
275	198	10	60	27.4	3001	PASS
365	198	1	100	1.3	140	PASS
441	198	0.01	100	13.4	1466	PASS
442	442	50	100	100.0	9085	PASS
443	442	15	24	18.4	1673	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073021\  
 Data File : BF124867.D  
 Acq On : 30 Jul 2021 8:40  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Jul 30 11:09:05 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF072221.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 22 15:28:57 2021  
 Response via : Initial Calibration

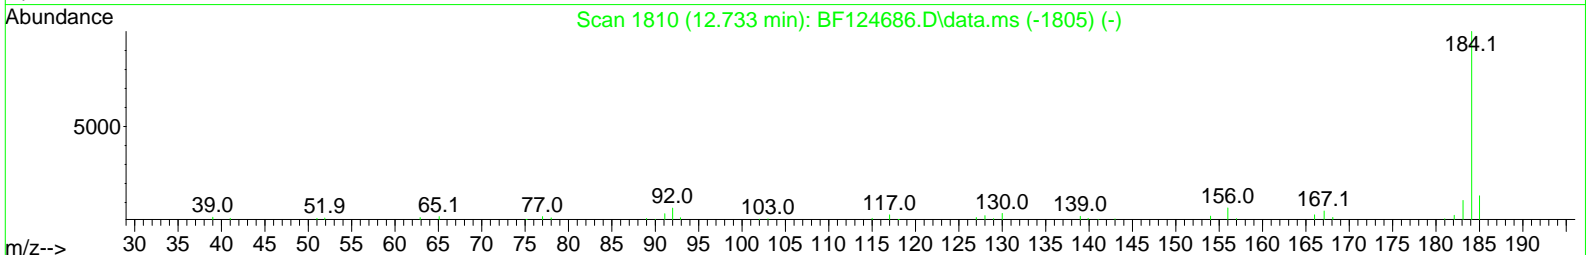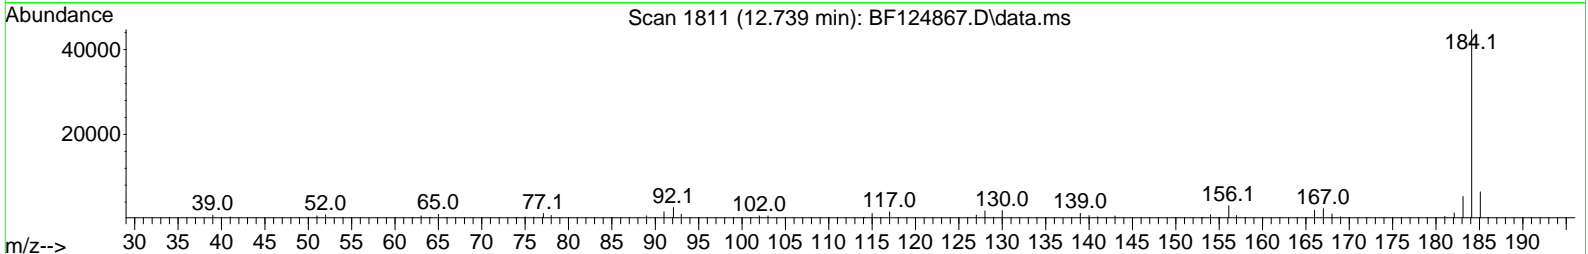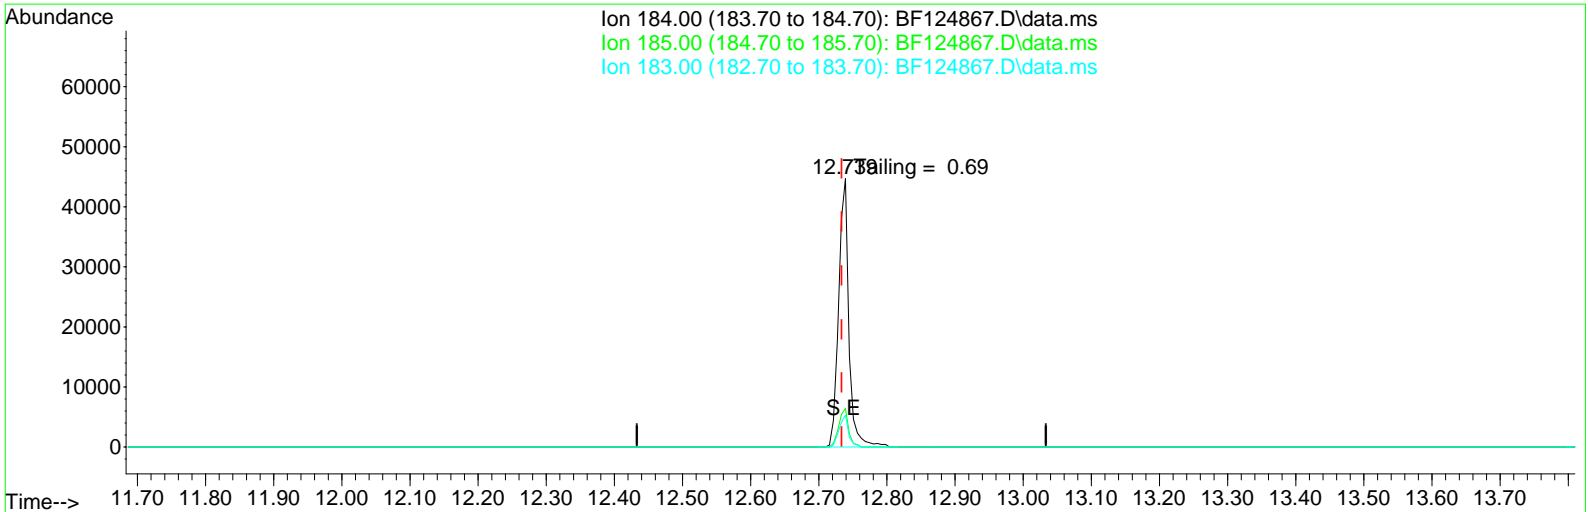

TIC: BF124867.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng




response 46757

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.40
183.00	10.10	11.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF073021\  
 Data File : BF124867.D  
 Acq On : 30 Jul 2021 8:40  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_F  
**ClientSampleId :**  
 DFTPP

Quant Time: Jul 30 11:09:05 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF072221.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 22 15:28:57 2021  
 Response via : Initial Calibration

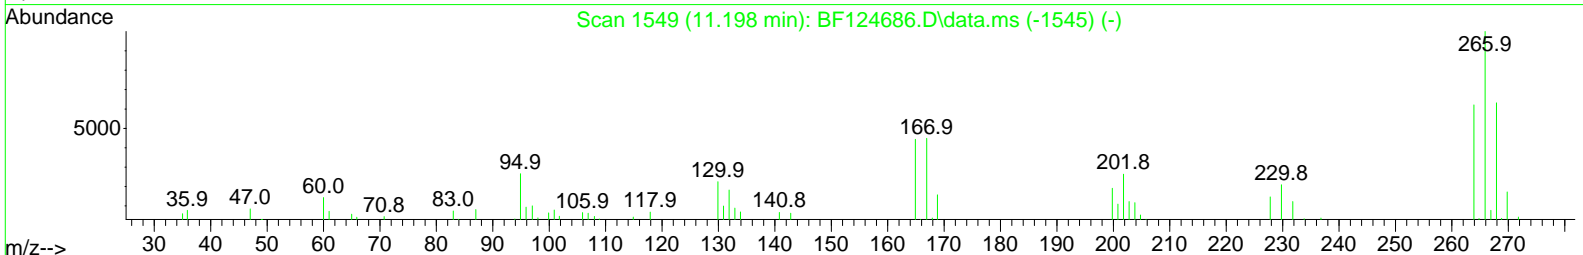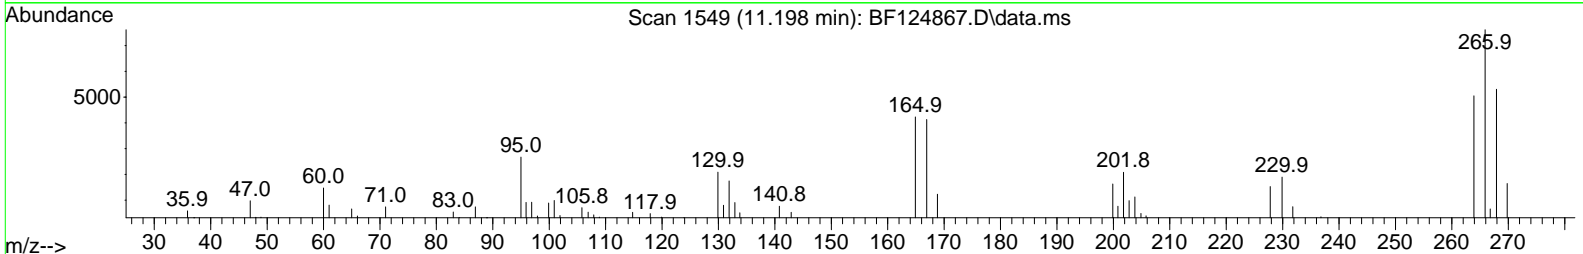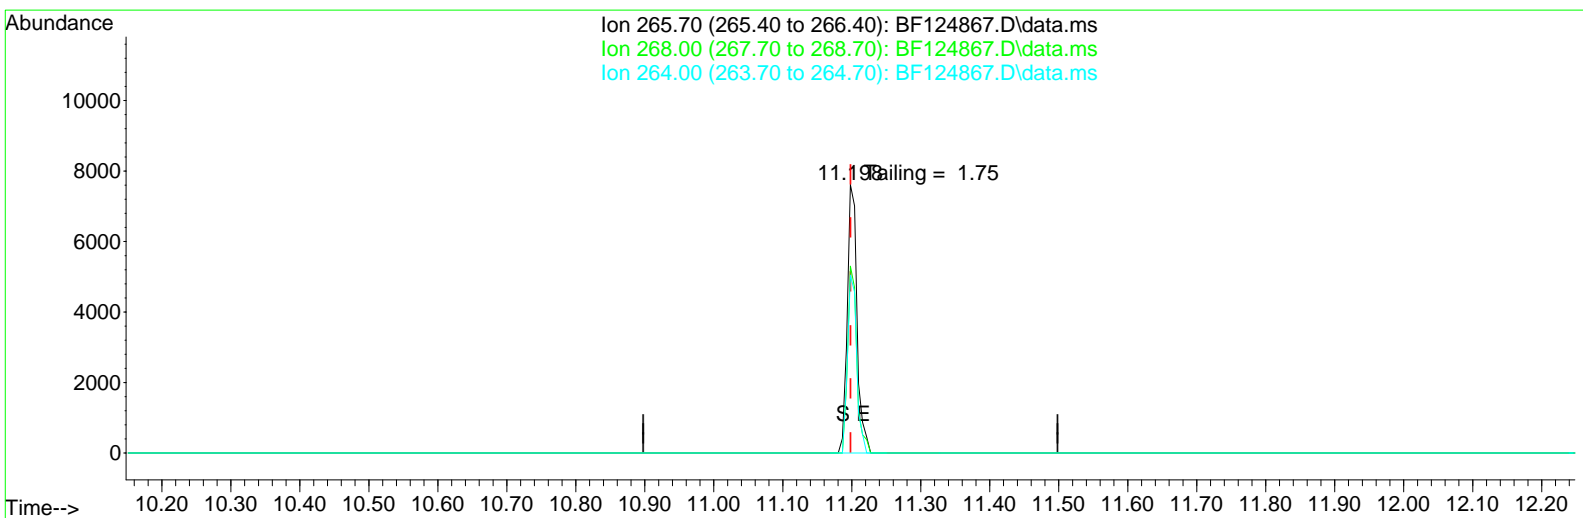

TIC: BF124867.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 0.00 ng

response	7508
Ion	Exp% Act%
265.70	100.00 100.00
268.00	61.10 69.65
264.00	69.90 66.32
0.00	0.00 0.00

**DDT Breakdown**

<b>Date</b>	<b>Instrument Name</b>	<b>DFTPP Data File</b>
7/30/2021	BNA_F	<u>BF124867.D</u>
<b>Compound Name</b>	<b>Response</b>	<b>Retention Time</b>
DDT	26479	13.55
DDD	350	13.25
DDE	0	12.71
<b>SUM(DDD+DDE)</b>	<b>SUM(DDT+DDD+DDE)</b>	<b>% Breakdown Of DDT</b>
350	26829	1.30