

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
 Data File : BF080751.D
 Acq On : 1 Aug 2015 00:00
 Operator : TP/UM
 Sample : G3125-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.224	6	12	15	rBV	9840	33254	2.15%	0.247%
2	4.384	199	201	206	rVB	54972	64043	4.14%	0.477%
3	5.024	255	257	260	rBV	803768	946113	61.11%	7.041%
4	5.447	291	294	296	rBV	768672	1082506	69.92%	8.056%
5	5.859	328	330	334	rVB	38883	33060	2.14%	0.246%
6	6.464	381	383	386	rBV	981001	952083	61.49%	7.086%
7	6.613	394	396	398	rBV	1240337	1086587	70.18%	8.087%
8	6.853	414	417	419	rBV	824603	751157	48.52%	5.590%
9	7.002	428	430	433	rBV	725596	762633	49.26%	5.676%
10	7.402	463	465	468	rBV	449423	587277	37.93%	4.371%
11	8.133	526	529	531	rBV	1056363	929168	60.01%	6.915%
12	9.208	620	623	625	rBV	1043993	865026	55.87%	6.438%
13	9.608	655	658	660	rBV	124055	174395	11.26%	1.298%
14	9.882	680	682	685	rBV	966177	924517	59.71%	6.880%
15	10.671	748	751	753	rBV2	343090	482962	31.19%	3.594%
16	11.368	809	812	814	rBV	783149	905853	58.51%	6.742%
17	11.894	856	858	860	rBV	26469	25556	1.65%	0.190%
18	12.945	948	950	953	rBV	1835214	1548265	100.00%	11.523%
19	13.985	1039	1041	1044	rBV	536462	666595	43.05%	4.961%
20	14.099	1046	1051	1053	rVV3	8953	21942	1.42%	0.163%
21	14.168	1055	1057	1064	rVB2	13730	26671	1.72%	0.198%
22	15.402	1162	1165	1168	rBV	423271	567201	36.63%	4.221%


Sum of corrected areas: 13436864

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
Data File : BF080751.D
Acq On : 1 Aug 2015 00:00
Operator : TP/UM
Sample : G3125-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

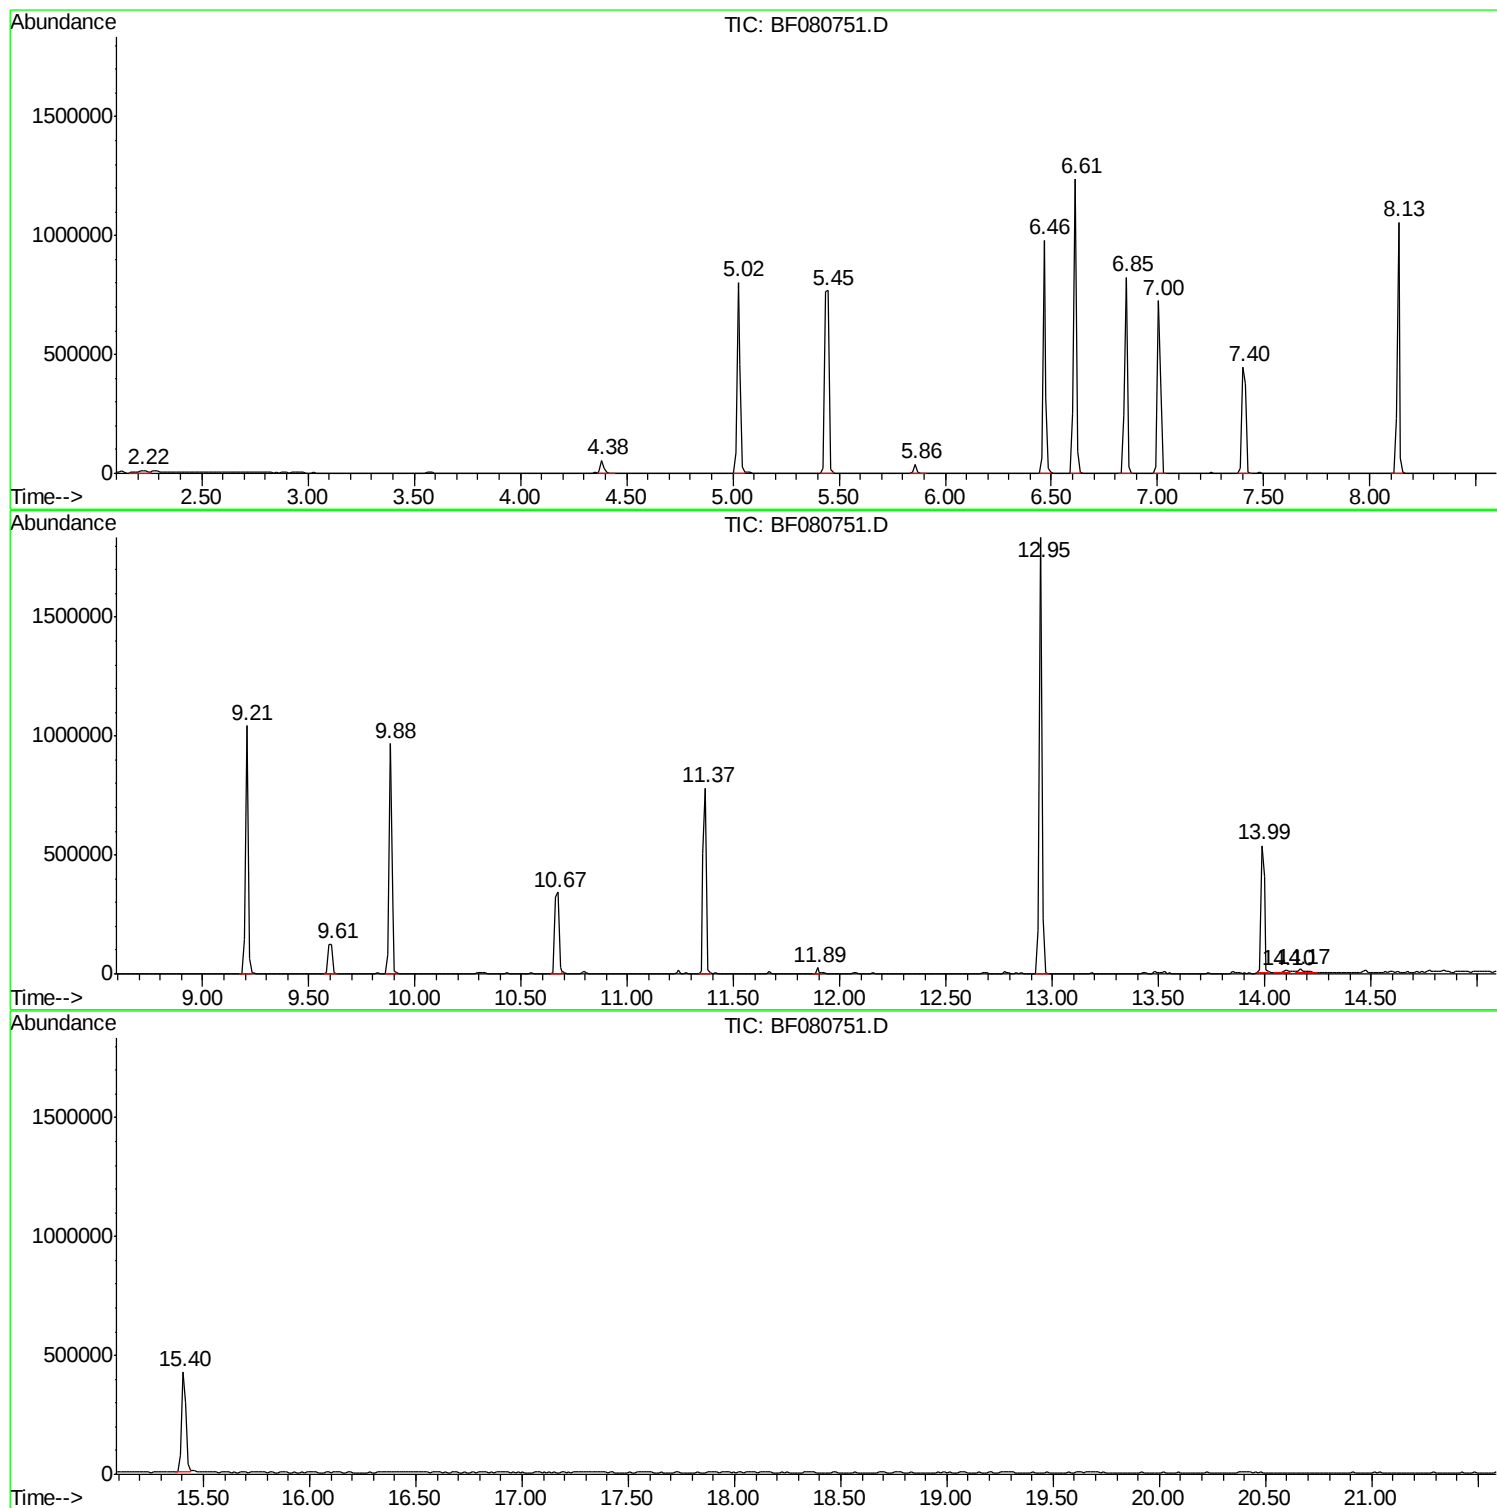

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
Data File : BF080751.D
Acq On : 1 Aug 2015 00:00
Operator : TP/UM
Sample : G3125-19
Misc :
ALS Vial : 43 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.02	25.19 ng	946113	1,4-Dichlorobenzene-d4	6.85	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32
5	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28

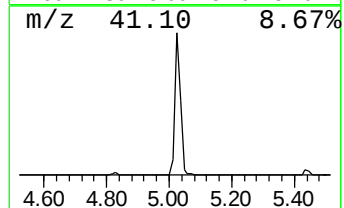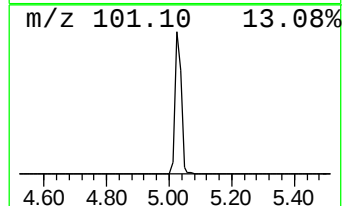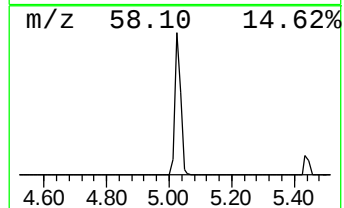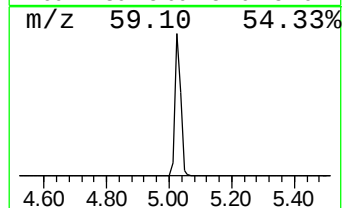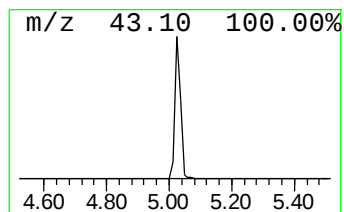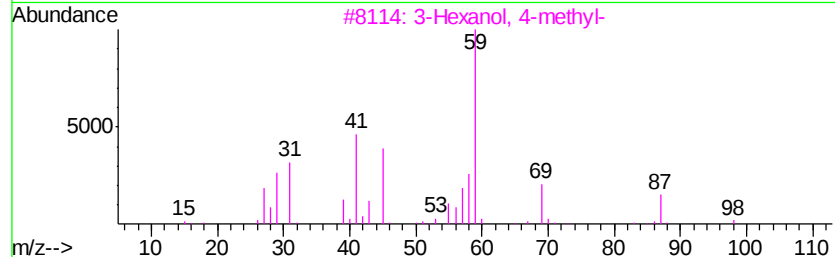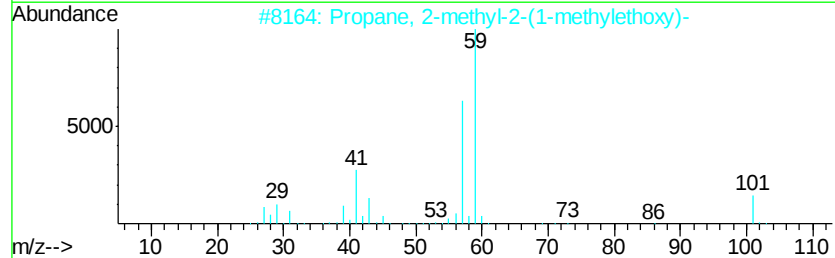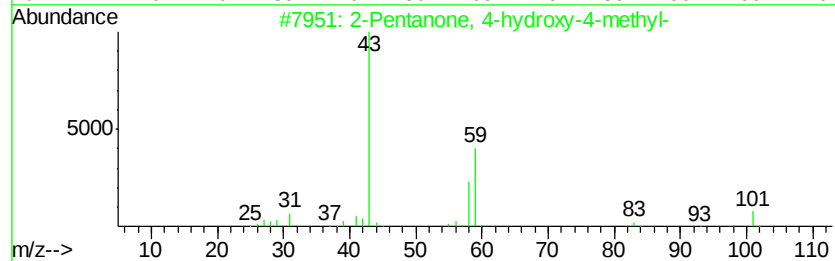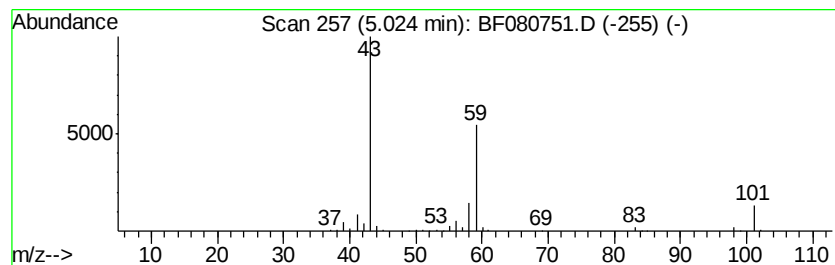

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
Data File : BF080751.D
Acq On : 1 Aug 2015 00:00
Operator : TP/UM
Sample : G3125-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	28.93 ng	1086590	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	25
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
5		1,2,3-Trifluorobenzene	132	C6H3F3	001489-53-8	9

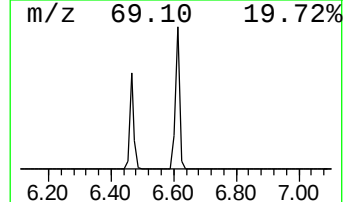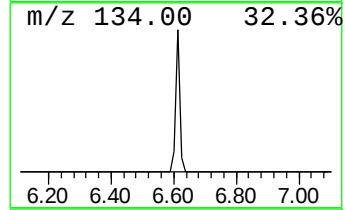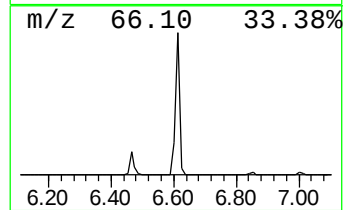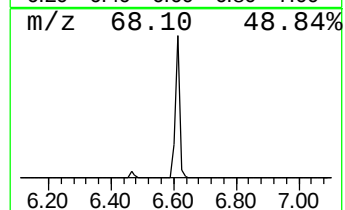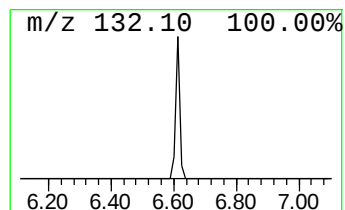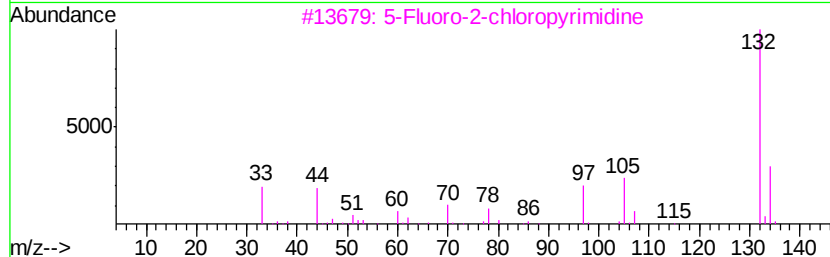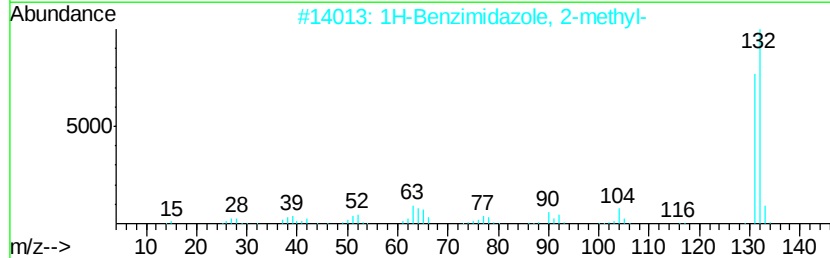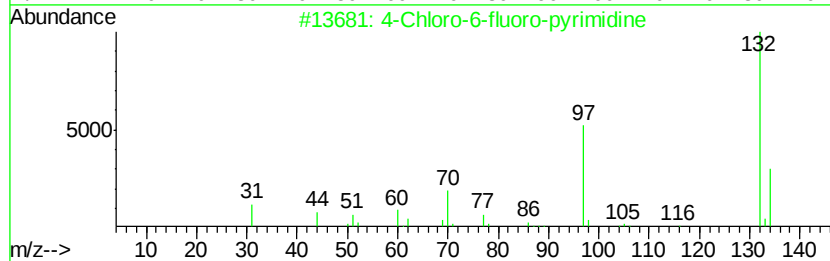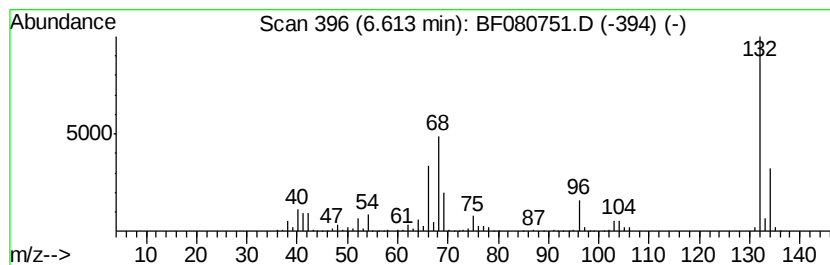

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
Data File : BF080751.D
Acq On : 1 Aug 2015 00:00
Operator : TP/UM
Sample : G3125-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.02	25.2	ng	946113	1	6.85	751157	20.0
unknown6.61	6.61	28.9	ng	1086590	1	6.85	751157	20.0