

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
 Data File : BF080758.D
 Acq On : 1 Aug 2015 3:35
 Operator : TP/UM
 Sample : G3115-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.315	18	20	22	rVB	8685002	11834148	100.00%	21.121%
2	3.538	124	127	134	rBV	69472	118677	1.00%	0.212%
3	4.441	203	206	208	rBV	1133006	1669863	14.11%	2.980%
4	5.081	258	262	264	rBV	2792738	4489466	37.94%	8.013%
5	5.470	293	296	299	rBV	3482462	3811685	32.21%	6.803%
6	5.870	329	331	334	rBV	192212	161860	1.37%	0.289%
7	6.487	381	385	387	rBV	3134548	4123301	34.84%	7.359%
8	6.624	394	397	399	rBV	4267689	4545418	38.41%	8.112%
9	6.853	415	417	419	rBV	1043913	872131	7.37%	1.557%
10	7.013	428	431	433	rBV	2874879	3282428	27.74%	5.858%
11	7.413	463	466	468	rBV	2886499	2948843	24.92%	5.263%
12	8.133	526	529	531	rBV	1191602	1107499	9.36%	1.977%
13	9.207	620	623	626	rBV	3729765	4774074	40.34%	8.521%
14	9.882	679	682	684	rBV	1166082	1135882	9.60%	2.027%
15	10.670	748	751	753	rBV	3284553	3384634	28.60%	6.041%
16	11.368	809	812	814	rBV	1006680	1189845	10.05%	2.124%
17	12.956	948	951	953	rBV	4469082	5122065	43.28%	9.142%
18	13.985	1039	1041	1044	rBV	617155	819543	6.93%	1.463%
19	15.402	1162	1165	1168	rBV	463607	639057	5.40%	1.141%


Sum of corrected areas: 56030419

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073115\
Data File : BF080758.D
Acq On : 1 Aug 2015 3:35
Operator : TP/UM
Sample : G3115-01
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

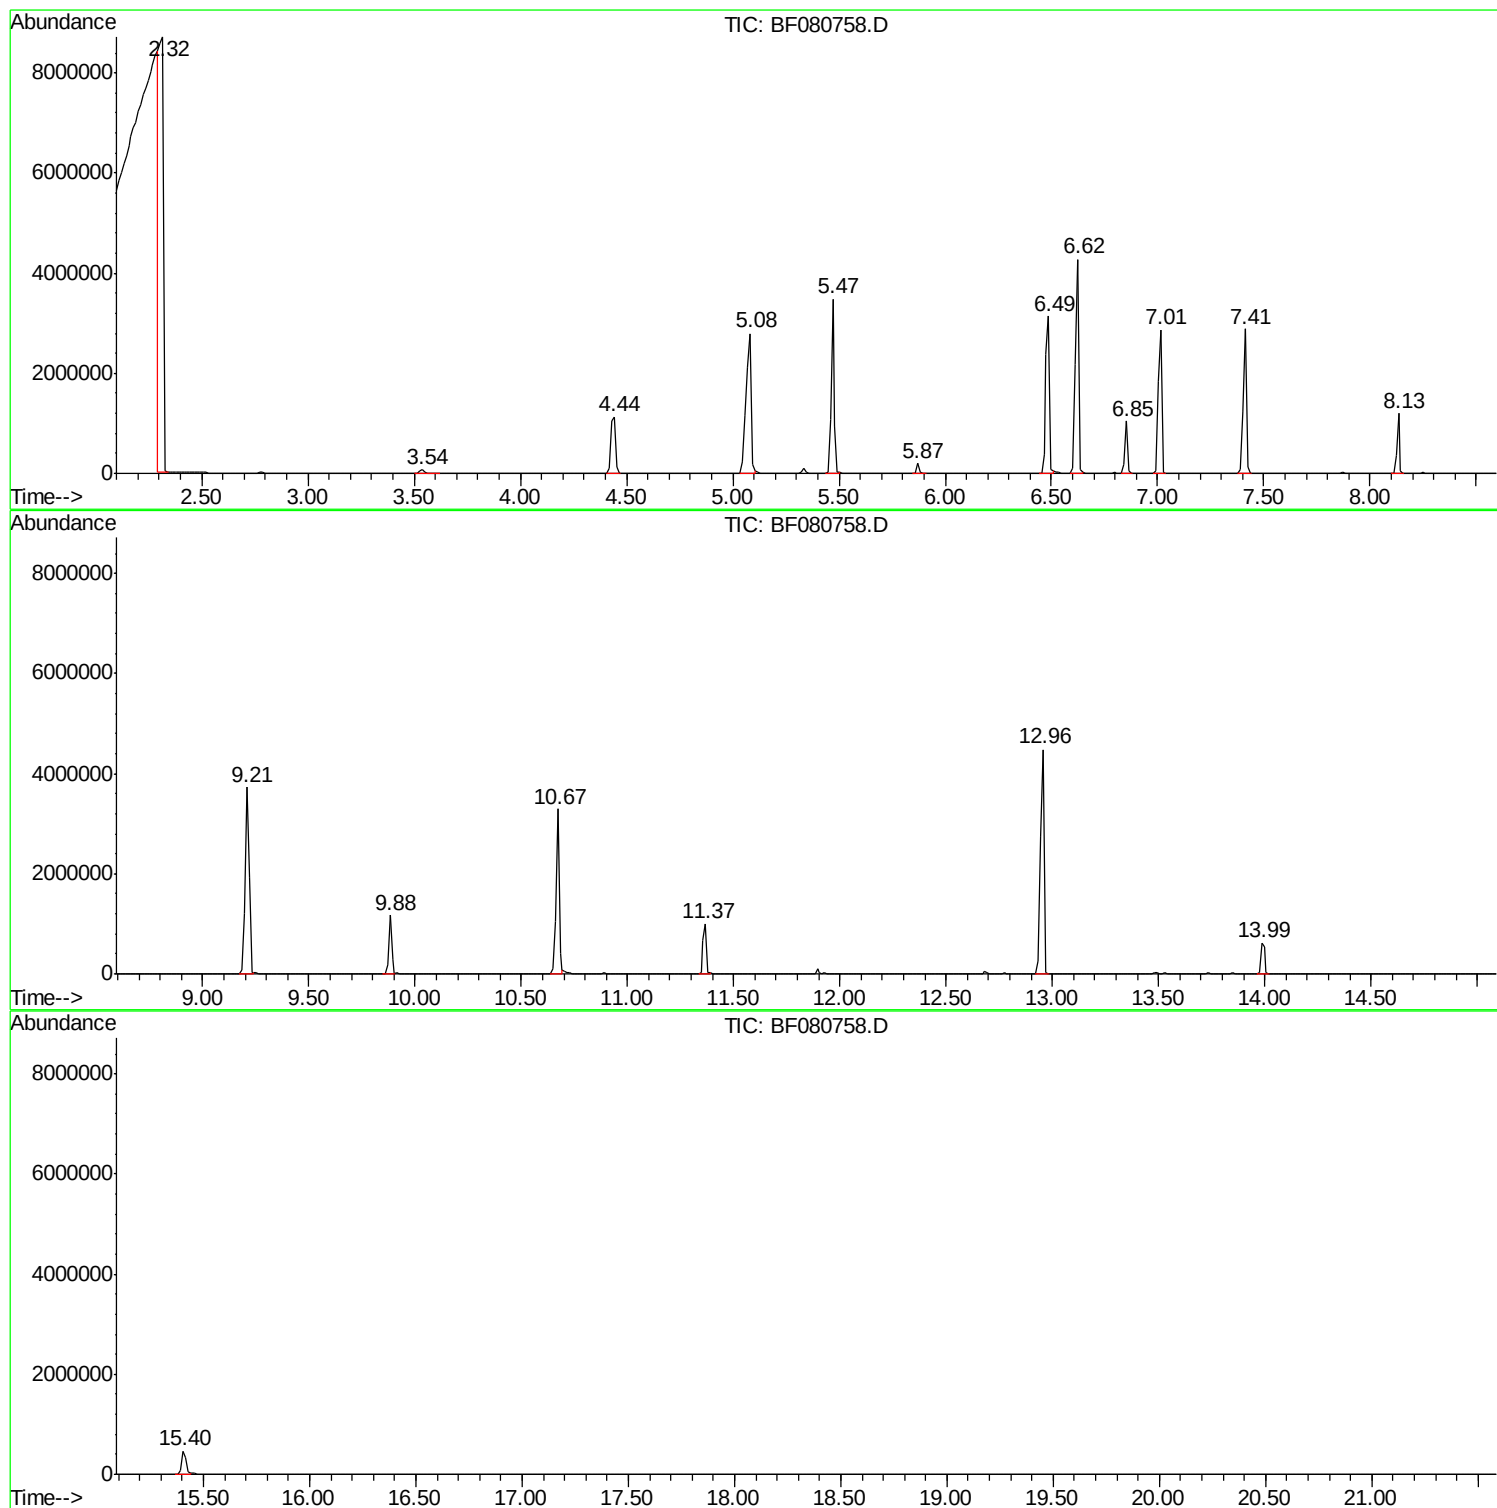

DbaaaPath::ZZ\NRPBMM\BNAF\DATA\B0033155\
 DbaaaFile::BB0000388DD
 AcqQOn :: 11Agg20055 3335
 Operator::TPPMM
 Sample::G0315001
 Misc ::
 ASSVal::500 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :

QcAntMebdd::ZZ\NRPBMM\BNAF\MEH00S8200BB003005MM
 QcAntTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary::CC\DATA\BBS6EN055002LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
