
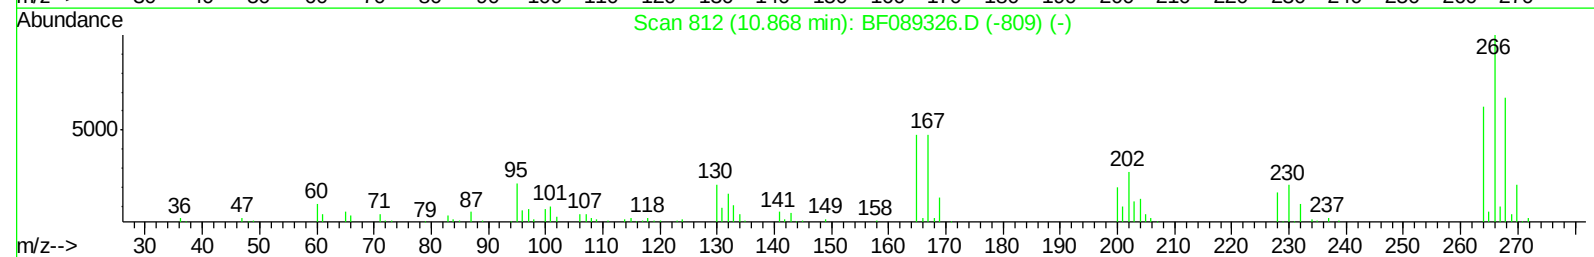
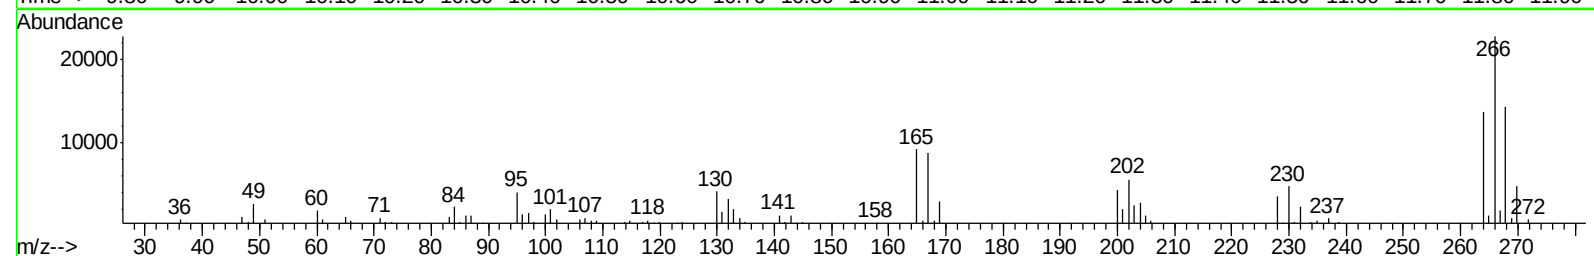


Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\
Data File : BF089448.D
Acq On : 30 Jul 2016 11:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:04:58 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

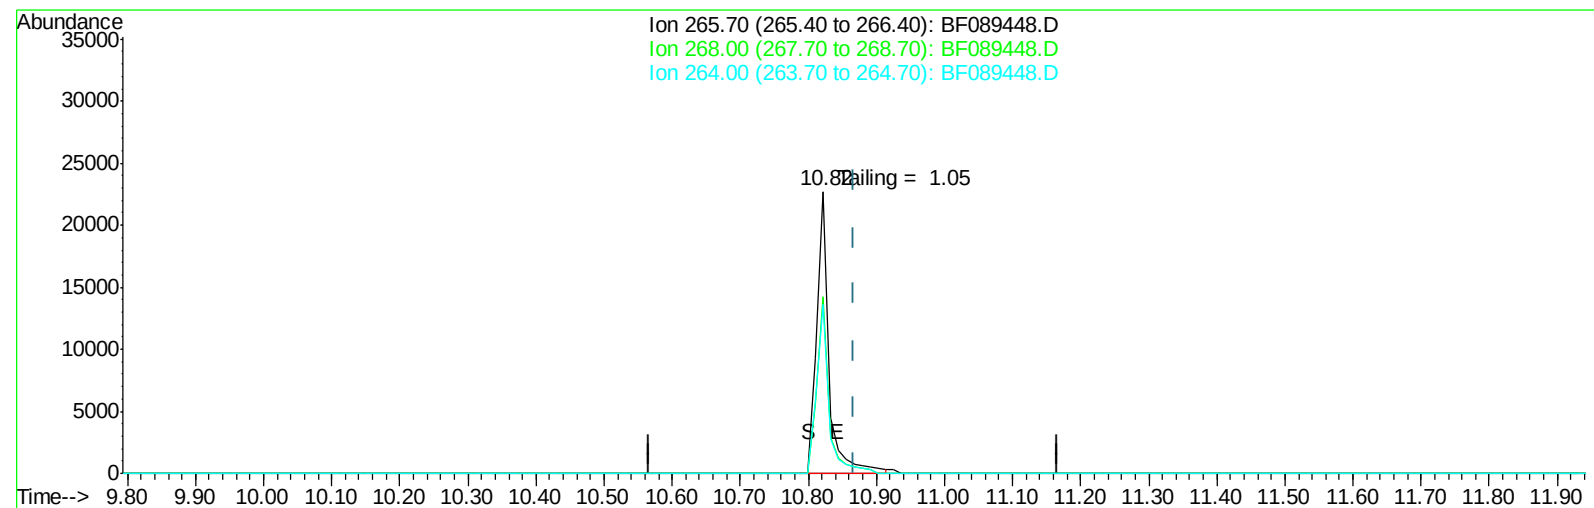

TIC: BF089448.D

(69) Pentachlorophenol (C)




10.822min (-0.045) 0.00ng

response 29112

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	62.61
264.00	62.70	59.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\
Data File : BF089448.D
Acq On : 30 Jul 2016 11:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:04:58 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

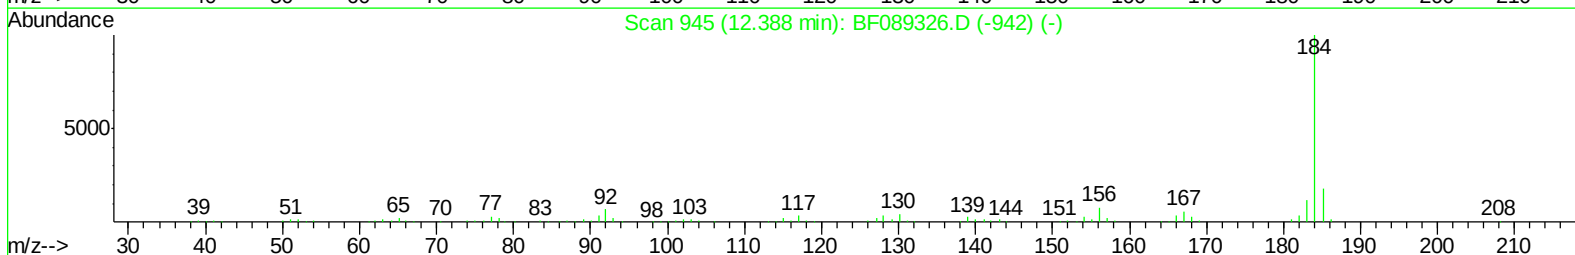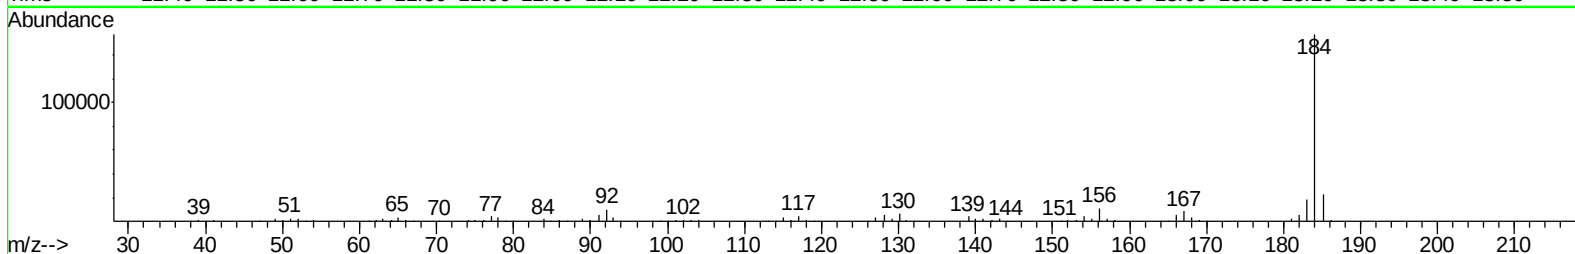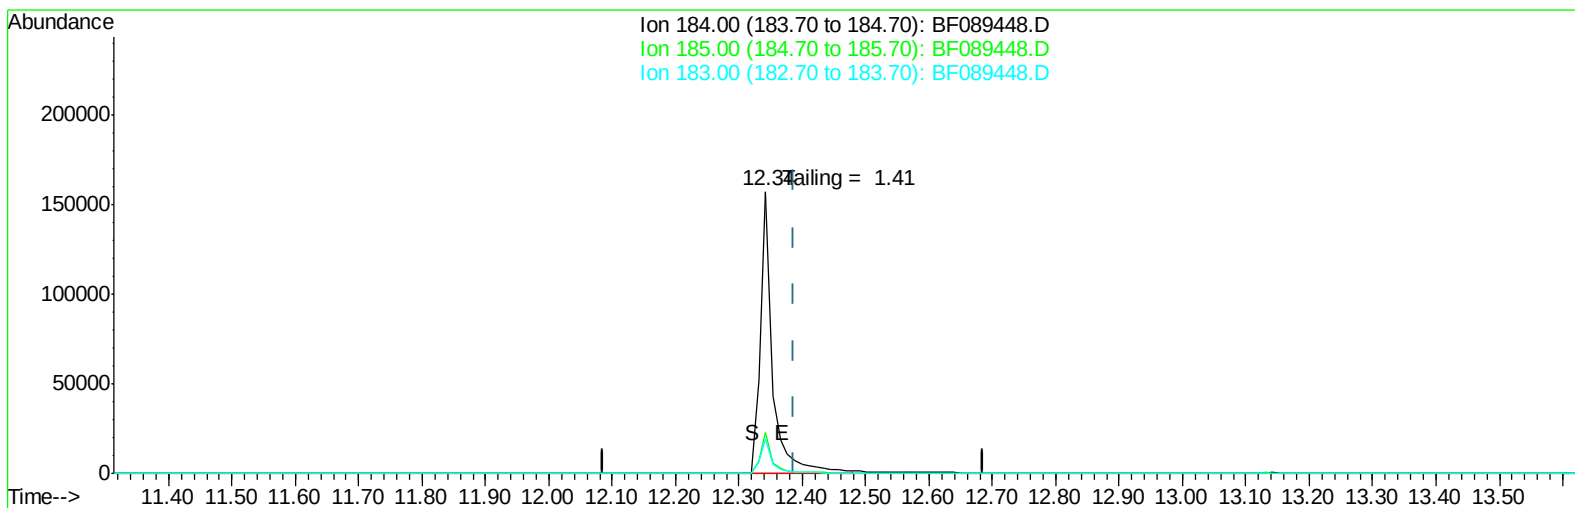

TIC: BF089448.D

(76) Benzidine

12.342min (-0.045) 0.00ng

response 220102

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	14.34
183.00	12.20	12.14
0.00	0.00	0.00