
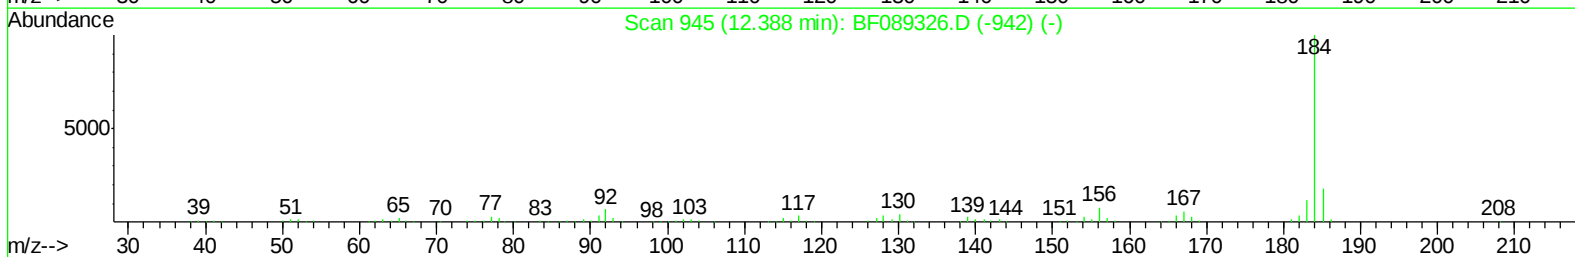
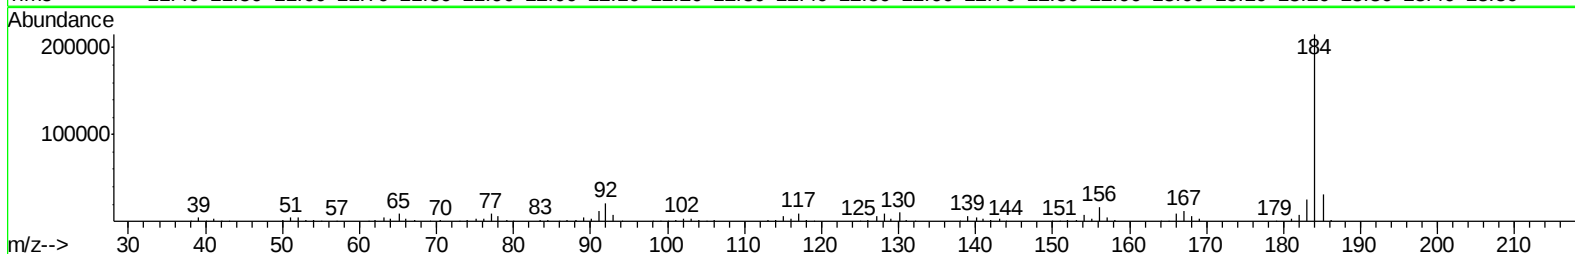


Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\
Data File : BF089464.D
Acq On : 31 Jul 2016 10:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:06:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

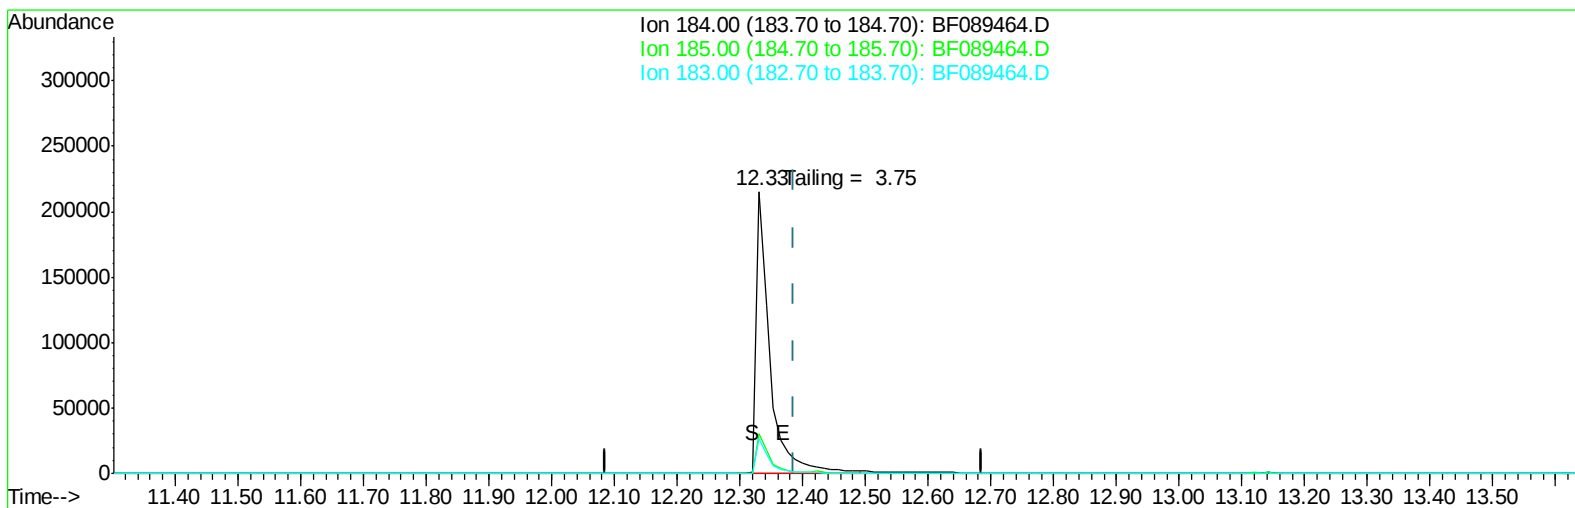

TIC: BF089464.D

(76) Benzidine




12.331min (-0.056) 0.00ng

response 337469

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	14.27
183.00	12.20	12.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\
Data File : BF089464.D
Acq On : 31 Jul 2016 10:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:06:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

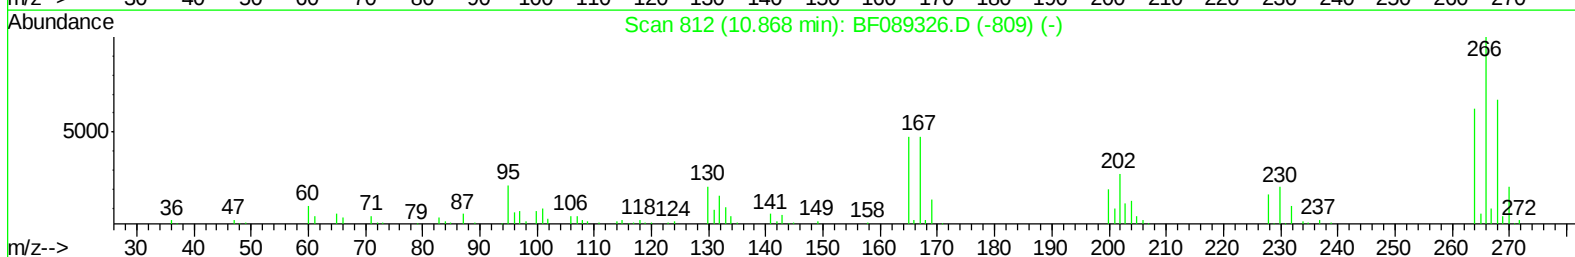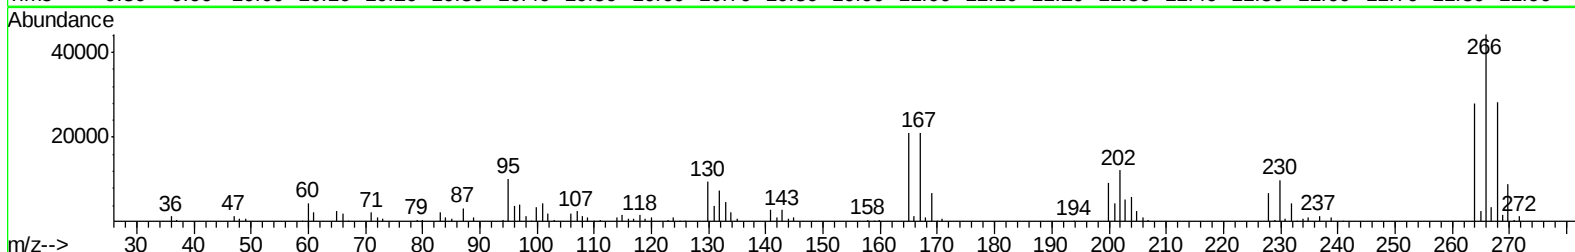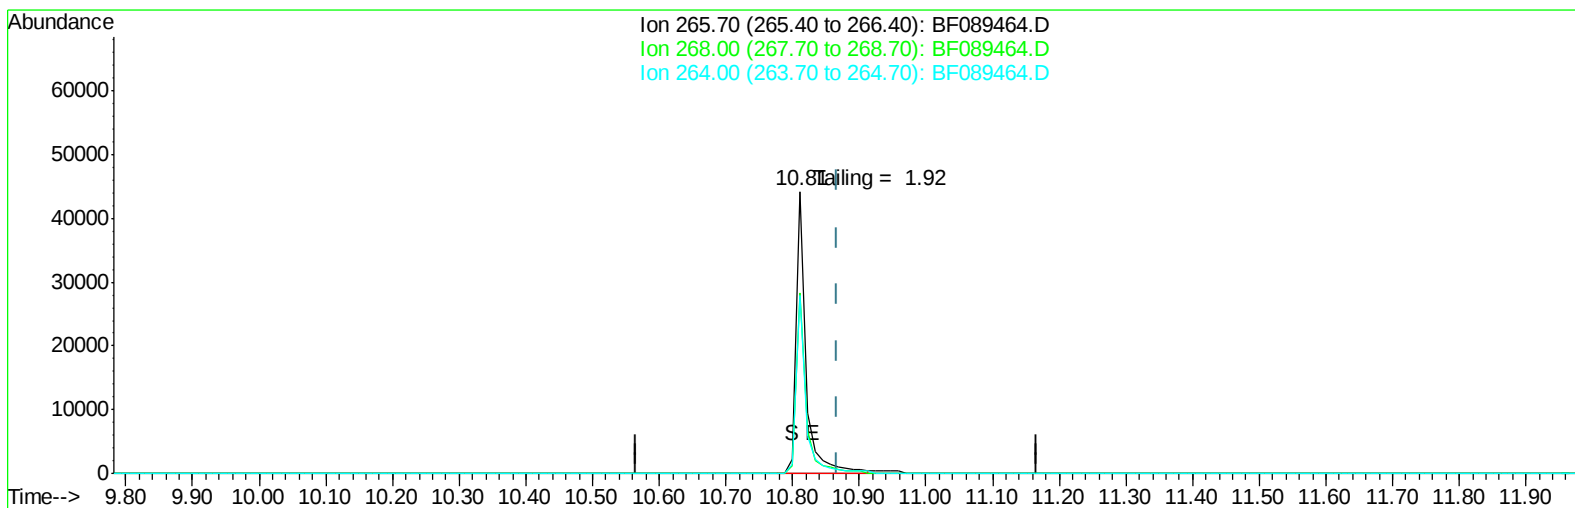

TIC: BF089464.D

(69) Pentachlorophenol (C)

10.811min (-0.056) 0.00ng

response 46379

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	64.24
264.00	62.70	63.26
0.00	0.00	0.00